

A

11/10/99

JC564 U.S. PTO

**IN THE UNITED STATES PATENT AND TRADEMARK OFFICE**

Atty. Docket: L-F / 168DV3

Applicant: Charles S. Neer, John N. Minnich


Title: MEDICAL FLUID INJECTOR HAVING FACE PLATE WITH MAGNETIC CONDUCTORS (As amended)

**CERTIFICATE OF MAILING BY EXPRESS MAIL - 37 CFR 1.10**

'Express Mail' mailing label number: EL420322646US

Date of Deposit: November 10, 1999

I certify that this paper or fee (along with the enclosures noted herein) is being deposited with the United States Postal Service 'Express Mail Post Office to Addressee' service under 37 CFR 1.10 on the above date and is addressed to the Assistant Commissioner for Patents, Washington, D.C. 20231

  
By: Heath R. Bandy (person mailing paper)

**UTILITY PATENT APPLICATION TRANSMITTAL**

***BOX PATENT APPLICATION***

*Assistant Commissioner for Patents  
Washington, D.C. 20231*

This is a request for filing, under 37 CFR § 1.53(b), a(n):

- ☐ Original (non-provisional) application.
- ☒ **Divisional of prior application Serial No. 09/189,470, filed on November 10, 1998, which is a divisional of prior application Serial No. 08/753,288, filed on November 22, 1996.**
- ☐ Continuation of prior application Serial No. \_\_, filed on \_\_.
- ☐ Continuation-in-part of prior application Serial No. \_\_, filed on \_\_.

For Divisional and Continuation applications ONLY:

- ☒ **Copy of Executed Declaration, Power of Attorney and Petition Form from parent application is enclosed (as noted below in Enclosures).**
- ☒ **Incorporation by Reference: The entire disclosure of the prior application, from which a copy of the oath or declaration is supplied herewith, is considered as being part of the disclosure of the accompanying application and is hereby incorporated by reference therein.**

For all Divisional, Continuation and Continuation-in-part applications:

- ☐ A Small Entity Statement was filed in the prior application, small entity status is still proper and desired.
- ☒ **This application is assigned to Liebel-Flarsheim Company by virtue of an earlier assignment filed in the prior application at Reel 8315, Frame 328-337.**
- ☒ **Please amend the application by inserting at page 1, line 1, "This application is a divisional of application serial no. 09/189,470, filed on November 10, 1998, which is a divisional of prior application Serial No. 08/753,288, filed on November 22, 1996."**
- ☒ **Please further amend the application title to: MEDICAL FLUID INJECTOR HAVING FACE PLATE WITH MAGNETIC CONDUCTORS.**

For all Divisional, Continuation and Continuation-in-part applications: (continued)

- ☒ Please note the inventors named in this application are fewer than those named in the prior application and the attached Declaration.

#### PRELIMINARY AMENDMENT/CALCULATION OF FEES

- ☒ Please cancel claims 1-32, 34-38 without prejudice, and prior to calculating the fees. 1 total claim(s), of which 1 is(are) independent, is(are) pending after the amendment.
- ☐ Please enter the enclosed preliminary amendment identified below prior to calculating the fees.     total claim(s), of which     is(are) independent, is(are) pending after the amendment.
- ☒ The Fees are Calculated as Follows:

Fee:	Number of Claims:	In Excess of:	Extra:	At Rate:	Amount:
Total Claims	1	20	0	\$18	\$0.00
Independent Claims	1	3	0	\$78	\$0.00
MULTIPLE DEPENDENT CLAIM FEE					
BASIC FEE					\$760.00
TOTAL OF ABOVE CALCULATIONS					\$760.00
REDUCTION BY 50% FOR FILING BY SMALL ENTITY					
TOTAL					\$760.00

#### ENCLOSURES

- ☒ Utility Patent Application Transmittal Form (in duplicate) containing Certificate of Mailing By Express Mail Under 37 CFR 1.10.
- ☒ Return Postcard.

#### APPLICATION PAPERS

- ☒ Utility Patent Application, with: cover sheet, 89 page(s) specification (including 38 total claim(s), of which 7 is(are) independent), and 1 page(s) abstract.
- ☒ Drawings: 13 sheet(s) of formal drawings ( 19 total figure(s)).
- ☐ Microfiche Computer Program (Appendix).
- ☐ Nucleotide and/or Amino Acid Sequence, including (all are necessary): Computer Readable Copy, Paper Copy (identical to computer copy), and Statement verifying identity of copies.
- ☐ An     Declaration, Power of Attorney and Petition Form.
- ☒ Copy of Executed Declaration, Power of Attorney and Petition Form from prior application identified above.
- ☐ Certified Copy of priority document(s) identified as attached above.

ADDITIONAL PAPERS

- ☐ Assignment to \_\_, Recordation Cover Sheet (Form PTO-1595)
- ☐ Verified Statement to Establish Small Entity Status under 37 CFR 1.9 and 1.27.
- ☐ Preliminary Amendment (to be entered prior to calculation of fees)
- ☒ Information Disclosure Statement, 5 sheet(s) Form PTO-1449, 0 U.S. Patent Reference(s),  
0 Foreign Patent Reference(s) and 0 Other Reference(s)
- ☐ Other: \_\_


CHECKS

- ☒ A Check of \$760.00 for the filing fee.
- ☐ A Check of \_\_ for the assignment recording fee.

DEPOSIT ACCOUNT AUTHORIZATION

- ☐ Please charge Deposit Account No. 23-3000 in the amount of \_\_.
- ☒ The Commissioner is authorized to charge any fees under 37 CFR 1.16 and 1.17 which may be required during the entire pendency of the application, or credit any overpayment, to Deposit Account No. 23-3000. A duplicate of this transmittal is attached.
- ☐ THE PAYMENT OF FEES IS BEING DEFERRED.

Respectfully Submitted,



Thomas W. Humphrey  
Reg. No. 34,353

WOOD, HERRON & EVANS, L.L.P.  
2700 Carew Tower  
Cincinnati, Ohio 45202  
(513) 241-2324

TWH/lgk

EXPRESS MAIL NO.: TB875323572US

APPLICATION  
FOR  
UNITED STATES LETTERS PATENT

TITLE: MEDICAL FLUID INJECTOR

APPLICANT: Dane J. Battiato, Gary S. Wagner, Steve P. Verdino,  
Robert G. Bergen, James E. Knipfer, Pamela K. Jacobs,  
Peter F. Staats, John N. Minnich, Charles S. Neer, James  
H. Goethel, Mitchell G. Stern

ASSIGNEE: LIEBEL-FLARSHEIM COMPANY

Wood, Herron & Evans, P.L.L.  
2700 Carew Tower  
Cincinnati, Ohio 45202

SPECIFICATION

6077 "OF 23460

## MEDICAL FLUID INJECTOR

### Abstract of the Disclosure

A medical fluid injector includes: an air detection system for detecting air in the neck of the syringe; a hand-operated control lever for controlling movement of the injector ram; magnetic conductors for delivering magnetic fields from a power head face plate to an internal circuit board to permit detection of different face plates; a tilt sensor detecting the tilt angle of the power head to control the speed of motion brought about by the hand-operated control lever and to control an invertible display; and a monitor microcontroller for monitoring the behavior of the central processing unit to detect and react to error conditions.

65074046

MEDICAL FLUID INJECTOR

Field of the Invention

5       The present invention relates to injectors  
for injecting fluid into animals.

Background of the Invention

10       In many medical environments, a medical  
fluid is injected into a patient during diagnosis or  
treatment. One example is the injection of contrast  
media into a patient to improve CT, Angiographic,  
Magnetic Resonance or Ultrasound imaging, using a  
powered, automatic injector.

15       Injectors suitable for these and similar  
applications typically must use a relatively large  
volume syringe and be capable of producing  
relatively large flow rates and injection pressures.  
For this reason, injectors for such applications are  
typically motorized, and include a large, high mass  
injector motor and drive train. For ease of use,  
20   the motor and drive train are typically housed in an  
injection head, which is supported by a floor, wall,  
or ceiling mounted arm.

      The injection head is typically mounted on  
the arm in a pivotal manner, so that the head may be

tilted upward (with the syringe tip above the  
remainder of the syringe) to facilitate filling the  
syringe with fluid, and downward (with the syringe  
tip below the remainder of the syringe) for  
5 injection. Tilting the head in this manner  
facilitates removal of air from the syringe during  
filling, and reduces the likelihood that air will be  
injected into the subject during the injection  
process. Nevertheless, the potential for  
10 accidentally injecting air into a patient remains a  
serious safety concern.

In addition to the injection head  
discussed above, many injectors include a separate  
console for controlling the injector. The console  
15 typically includes programmable circuitry which can  
be used for automatic, programmed control of the  
injector, so that the operation of the injector can  
be made predictable and potentially synchronized  
with operations of other equipment such as scanners  
20 or imaging equipment.

Thus, at least part of the injection  
process is typically automatically controlled;  
however, the filling procedure, and typically some

part of the injection procedure, are normally performed by an operator, using hand-operated movement controls on the injector head. Typically, the hand-operated movement controls include buttons for reverse and forward movement of the injector drive ram, to respectively fill and empty the syringe. In some cases, a combination of buttons is used to initiate movement of the ram or to control ram movement speed. The injector head also typically includes a gauge or display for indicating injection parameters to the operator, such as the syringe volume remaining, for the operator's use when controlling the injector head. Unfortunately, operators have found it cumbersome to use the hand-operated movement buttons and to read the injector head gauges and displays, for several reasons, not the least of which is the necessary tilting of the injector head between the upward, filling position to the downward, injection position, changing the positions of the hand-operated movement buttons relative to the operator, and at some tilt angles rendering the gauges or displays difficult to read.

In many applications, it is desirable to use an injector with multiple different syringe sizes. For example, it may be desirable to use a smaller syringe for pediatric use than for adult use. To facilitate the use of different syringe sizes, injectors have been constructed with removable face plates, where each of the various face plates is configured for a particular syringe size. Typically, the injector is able to adjust injection parameters by detecting which face plate is mounted to the injector, for example using a magnetic detector mounted to the front surface of the injector housing to detect the presence or absence of a magnet in the face plate.

Unfortunately, the necessity of incorporating a magnetic detector into the outer housing of the injector head increases the complexity and expense of manufacturing the injector head.

#### Summary of the Invention

In accordance with the invention, improvements are made on these various aspects of the operation of the typical injector.

In particular, an injector in accordance with the invention features an air bubble detection system positioned adjacent the tip of the syringe for detecting the presence of air in the tip of the syringe. This detection system, which is electrically connected directly to the control circuitry in the injector, permits the injector to detect air in the tip of the syringe, and if air is detected, to halt any prospective or ongoing injection. Since air is detected prior to exit from the syringe and before passage through the tubing leading to the patient, rather than at some intermediate point along the tubing, the injector is more likely to detect air early enough to prevent or halt the injection before the air reaches the patient.

In the specific disclosed embodiment, the air detector generates a light beam and directs this light beam into the tip of the syringe, where it is reflected from the inner wall of the syringe tip and returned into a detector. Other methods of air detection, such as ultrasonic air detection, may also be performed by a detector mounted at the

syringe tip with similar advantage, and are encompassed within the scope of the invention.

Another aspect of this feature of the injector is the structure of the syringe tip, which includes an outwardly-projecting transparent section positioned for mechanical coupling to the source of light in the air detector, to facilitate light coupling into the syringe tip for reflection from the inner wall of the tip and return to the detector. This outwardly-projecting section forms a lens for focusing light impinging upon the syringe tip so that this light properly reflects through the interior of the syringe tip.

The injector in accordance with the present invention also features a hand-operated fill/expel control which facilitates operator control of the injector. The control includes a lever movable between home, forward, and reverse positions, where movement of the lever to the forward position causes the injector to move the plunger drive ram forward to expel fluid from the syringe, and movement of the lever to the reverse

position causes the injector to move the plunger  
drive ram in reverse to draw fluid into the syringe.

In specific embodiments, the lever is  
mounted on a pivot, and biased to the home position  
5 by return springs positioned on opposite sides of  
the lever. Rotation of the lever away from the home  
position progressively bends the springs at  
increasing angles of lever rotation. A detector,  
specifically a rotary potentiometer, detects the  
10 angle of rotation of the lever, so that this angle  
can be used to control the speed of motion of the  
plunger drive ram. Using this structure and  
control, the relative position of the lever, and (if  
desired) the return torque applied by the springs to  
15 the lever, can be made roughly proportional to the  
flow rate of fluid into or out of the syringe,  
providing the operator with intuitive feedback on  
the operation of the injector. Alternatively, the  
injector may control the injection pressure produced  
20 by the injector in response to the angle of rotation  
of the lever, to provide the operator with feedback  
on the injection pressure being applied.

As a safety feature, in the disclosed  
specific embodiment, the return springs and lever  
are elements in an electrical circuit which produces  
a movement control signal. The central processing  
5 unit controlling the injector responds to this  
signal by displaying a fault message, or rendering  
the hand-operated movement control inoperative, if  
one of the springs breaks, so that in such a case  
the injector will not respond to unintentional  
10 displacement of the lever away from the home  
position which might result from breakage of a  
spring.

As an aid in filling the syringe, an  
additional detent spring is positioned relative to  
15 the lever in order to alter the return torque  
applied to the lever when the lever is rotated more  
than a given angle away from the home position. The  
result is a "detent" that can be identified by the  
operator, i.e., an angle at which the resistive  
20 torque increases dramatically. This detent angle  
can have any desired significance, but in the  
disclosed embodiment, this angle of rotation  
corresponds to a recommended maximum speed for

filling the syringe, i.e. the largest speed at which  
fluid can be drawn into the syringe without dramatic  
increase in the generation of air bubbles. As with  
the other springs, the detent spring can be an  
5 electrical contact, used to produce a second control  
signal indicating that the lever has been rotated to  
the detent angle, so that the injector control  
circuitry can calibrate the speed at the moment the  
lever contacts the detent spring so that this lever  
10 position corresponds to the recommended maximum  
speed. Alternatively, the second control signal can  
be used to prevent the operator from attempting to  
fill the syringe at any faster rate.

To complement the intuitive feedback  
15 obtained from the above-described fill/expel lever,  
the injector in accordance with the present  
invention further features a tilt-compensating  
display. The injector head includes a tilt angle  
sensor for detecting the tilt angle of the head, and  
20 uses this tilt angle to choose one of two display  
orientations. As a result, the display is always  
oriented properly for reading by the operator,

regardless of whether the injector is tilted upright  
for filling or down for injection.

In the specific disclosed embodiment, the  
display is a light emitting diode display having  
5 elements arranged so that the display can provide  
the same information in either an upright or  
inverted orientation. However, other embodiments  
are contemplated, such as the use of a liquid  
crystal display, or a pixilated display permitting  
10 full variation in display attributes and  
orientations.

As further aspects of this feature, the  
tilt-sensing circuitry in the injector is also used  
to ensure proper operation of the injector. For  
15 example, the range of fill and expel speeds  
available from the hand-operated movement control is  
broader when the injector head is tilted upward than  
when the head is tilted downward. Furthermore, the  
injector prevents automatic injection unless the  
20 injector head is tilted downward, and/or the  
injector warns the operator of possible air  
injection when the head is not tilted at a  
sufficient downward angle.

600104000

The injection head in accordance with the invention has a compact, modular design facilitating manufacture and service. In particular, to the extent possible all control circuitry has been

5 incorporated onto a single printed circuit board. Notably, one feature of the inventive injector is the use of magnetic conductors to channel magnetic field energy from magnets positioned in the injector face plate, through the injector housing and into

10 the vicinity of magnetic detectors (e.g., Hall effect switches) mounted on the main circuit board. By using magnetic conductors to carry magnetic fields through the injector housing, circuit-board-mountable magnetic detectors can be used,

15 substantially reducing the overall cost as compared to purchasing individually packaged detectors for mounting in the injector housing.

In addition to the safety features identified above, the injector in accordance with

20 the present invention includes a hardware safety feature for detecting processor or software failures and preventing erroneous injections. Specifically, the injector head includes a central processing unit

for controlling all functions of the injector head,  
and a monitor microcontroller for monitoring the  
operation of the central processing unit. The  
central processing unit delivers information on its  
5 state of operation to the monitor microcontroller.  
The monitor microcontroller also monitors the hand-  
operated controls on the injector head and the  
movements of the injector drive ram to confirm that  
these controls and movements are consistent with the  
10 processor state reported by the central processing  
unit. If the two do not agree, the monitor  
microcontroller can halt operation of the injector  
head.

In the specific disclosed embodiment,  
15 there are central processing units in each of the  
injector head, console and power pack, which  
communicate with each other to operate the injector  
in its various modes, and each central processing  
unit is associated with a monitor microcontroller,  
20 and the monitor microcontrollers similarly  
intercommunicate to ensure that the central  
processing units are functioning correctly  
individually and collectively.

The above and other features, aspects, objects and advantages of the present invention shall be made apparent from the accompanying drawings and the description thereof.

5     Brief Description of the Drawing

          The accompanying drawings, which are incorporated in and constitute a part of this specification, illustrate embodiments of the invention and, together with a general description  
10     of the invention given above, and the detailed description of the embodiments given below, serve to explain the principles of the invention.

          Fig. 1 is a perspective view of an injector in accordance with principles of the  
15     present invention, including a power head, console, and power pack (under a cover), with the syringe, pressure jacket, heater blanket and air detection module removed;

          Fig. 2 is a perspective view of the power  
20     head of the injector of Fig. 1 with a pressure jacket, syringe and heater blanket mounted thereto, showing the power head display, hand-operated control, and support arm mounting in greater detail;

Fig. 3 is a disassembled view of the internal structure of the power head of Fig. 2 illustrating details of the face plate, circuit board, plunger ram drive and housing;

5            Fig. 4 is a partial sectional view of the internal structure of an assembled power head, taken along lines 4-4 in Fig. 3;

10           Fig. 5 is a partial sectional view taken along lines 5-5 of Fig. 4, showing the relative positions of the circuit board, housing, display and magnetic conductors within the housing;

Fig. 6 is a perspective, partial sectional view of the hand-operated control assembly;

15           Fig. 7A is a cross-sectional view of the hand-operated control assembly of Fig. 6 taken along lines 7A-7A of Fig. 6, showing the return and detent springs;

20           Fig. 7B is a cross-sectional view of the hand-operated control assembly showing the hand-operated control lever displaced from the home position and into contact with the detent spring;

Fig. 7C is an electrical schematic diagram of the electrical circuit formed by the hand-operated control lever, return and detent springs;

Fig. 8 is a perspective drawing of the heater blanket used to warm fluid in the syringe mounted to the injector;

Fig. 9 is a partial cross-sectional view of a syringe mounted in the pressure jacket with the air detection module in place, showing the internal structure of the air detection module and its interaction with the structure of the syringe tip;

Fig. 10 is a view of the air detection module taken along lines 10-10 of Fig. 9, with the syringe and pressure jacket removed;

Fig. 11A is an electrical block diagram illustrating the analog circuitry in the power head, including the temperature control, air detection, and hand-operated control circuitry;

Fig. 11B is an electrical block diagram of the digital control circuitry in the power head, including the central processing unit, monitor microcontroller, digital status, control and interface connections;

Fig. 11C is an electrical block diagram of the central processing units and microcontrollers in the power head, power pack and console and their interconnection;

5                    Fig. 12 illustrates the heater blanket temperature control methodology used by the CPU of the power head;

                  Fig. 13A illustrates the ranges of tilt angle established by software in the power head microprocessor to control operations of the  
10                   injector, Fig. 13B illustrates the elements in the display on the power head, and a typical display output as it would appear when the power head is at a first tilt angle, and Fig. 13C illustrates the  
15                   display output of the same information as Fig. 13B, as it would appear when the power head is at a second tilt angle.

#### Detailed Description of Specific Embodiments

                  Referring to Fig. 1, an injector 20 in  
20                   accordance with the present invention includes various functional components, such as a power head 22, a console 24 and power pack 26 (mounted inside of a cover). A syringe 36 (Fig. 2) is mounted to the

injector 20 in the face plate 28 of the power head  
22, and the various injector controls are used to  
fill the syringe with, e.g., contrast media for a  
CT, Angiographic or other procedure, which media is  
5 then injected into a subject under investigation  
under operator or pre-programmed control.

The injector power head 22 includes a  
hand-operated movement control lever 29 for use in  
controlling the movement of the internal drive  
10 motor, and a display 30 for indicating to the  
operator the current status and operating parameters  
of the injector. The console 24 includes a touch  
screen display 32 which may be used by the operator  
to remotely control operation of the injector 20,  
15 and may also be used to specify and store programs  
for automatic injection by the injector 20, which  
can later be automatically executed by the injector  
upon initiation by the operator.

Power head 22 and console 24 connect  
20 through cabling (not shown) to the power pack 26.  
Power pack 26 includes a power supply for the  
injector, interface circuitry for communicating  
between the console 24 and power head 22, and

66011-074650

further circuitry permitting connection of the injector 20 to remote units such as remote consoles, remote hand or foot control switches, or other original equipment manufacturer (OEM) remote control connections allowing, for example, the operation of injector 20 to be synchronized with the x-ray exposure of an imaging system.

Power head 22, console 24 and power pack 26 are mounted to a carriage 34 which includes a support arm 35 for supporting power head 22 for easy positioning of power head 22 in the vicinity of the examination subject. Other installations are also contemplated however; for example, console 24 and power pack 26 may be placed on a table or mounted on an electronics rack in an examination room while power head 22 is supported by a ceiling, floor or wall mounted support arm.

Referring now to Fig. 2, in operation, a syringe 36 and pressure jacket 38 are mounted to power head 22, so that the motor internal to power head 22 may be energized to move a plunger 37 within the barrel of syringe 36 toward and away from a discharge tip 40 of the syringe, to thereby expel

fluid from the syringe 36 or fill the syringe with fluid. Pressure jacket 38 provides support to the outer walls of syringe 36 to protect the walls of syringe 36 from failure at high injection pressures.

5                   Syringe 36 and pressure jacket 38 are made of a clear plastic material through which the operator can view the current location of plunger 37 and any fluid or air in the syringe between plunger 37 and discharge tip 40. Accordingly, as described  
10                   above, an operator may tilt power head 22 upward, fill syringe 36 from a source of fluid while visually monitoring the filling process, then connect the injector to tubing leading to the patient, expel air from the tubing and syringe while  
15                   visually monitoring the level of fluid in the syringe, and then once air has been expelled, tilt the injector downward and proceed to inject fluid into a subject.

                  To facilitate this filling process, and  
20                   other operations that may be performed during injection of a subject, power head 22 includes the hand-operated movement control, which is in the form of the rotatable lever 29. Specifically, lever 29

is rotatable on an axis of rotation inside of power head 22. When the hand-operated control lever 29 is left in its home position, illustrated in Fig. 2, no plunger motion is generated by power head 22.

5 However, when hand-operated control lever 29 is rotated toward syringe 36, forward plunger motion is generated by power head 22, expelling fluid or air from syringe 36. Alternatively, when hand-operated control lever 29 is rotated away from syringe 36,  
10 reverse plunger motion is generated by power head 22, filling syringe 36 with fluid or air. Further details on the construction and operation of hand-operated control lever 29 will be elaborated below in connection with Figs. 6-7C.

15 To ensure that fluid injected into a subject is maintained at approximately body temperature, a heater blanket 42 is installed abutting the exterior wall of pressure jacket 38. Heater blanket 42 includes an electrical heater  
20 which generates heat for regulating the temperature of fluid within syringe 36. Heater blanket 42 (which is separately illustrated in Fig. 8) is mounted to a post 44 extending from face plate 28,

holding heater blanket 42 in thermal contact with pressure jacket 38.

At the rear end of power head 22 is an indicator lamp 46 (covered by a light-diffusing cover) which indicates the status of the power head, as discussed in further detail below.

Now referring to Fig. 3, the internal structure of the power head 22 can be described.

Power head 22 is constructed from two external half-housings 47a and 47b. Half-housings 47a and 47b mate to form the complete housing for power head 22. The upper half-housing 47a includes an aperture through which the display 30 can be viewed, the indicator lamp 46, and bearing surfaces for supporting a shaft 48 to which hand-operated control lever 29 is attached. Details of the hand-operated control lever structure mounted internally to upper half-housing 47a are discussed in further detail below.

Lower half-housing 47b includes an aperture through which a knob 49 is mounted and coupled to the internal drive train. Knob 49 can be rotated by hand to move the drive train of the

plunger drive ram, to allow precise control of ram movements, and also to permit movement if an electrical failure disables the power head 22. A second aperture 51 in lower half-housing 47b is used to connect the power head circuit board 55 (see below) to electrical lines leading from the heater blanket 42 (see Figs. 2, 8) and air detector attachment (see Figs. 9, 10).

Lower half-housing 47b further includes a mounting track (opposite to indentation 50 inside of half-housing 47b) for receiving a mount 52 for supporting half-housing 47b on an articulated arm such as arm 35 shown in Figs. 1 and 2. Mount 52 may be inserted into the mounting track of lower half-housing 47b from either side of power head 22, facilitating mounting of power head 22 on either side of an examination table. A knob 53 holds mount 52 in place in the mounting track in lower half-housing 47b.

Internal features of power head 22 include a circuit board 55 which supports substantially all of the electrical circuitry for controlling the operations of power head 22. Notable components

found on circuit board 55 include magnetic detectors  
56a, 56b and 56c and flag sensor 58. The main  
circuit board also includes the indicator lamp 46  
(not shown). The functions of detectors 56a, 56b  
5 and 56c and flag sensor 58 will be elaborated more  
fully below.

Mounted below circuit board 55 inside of  
power head 22, is the drive train 60 for the plunger  
drive ram 62. Drive train 60 includes a rotary  
10 electric motor 63, controlled by circuit board 55,  
which (via a gear box 68) rotates a drive pinion 64.  
Pinion 64 meshes with a main gear 65, which rotates  
a ball screw 66. Plunger drive ram 62 is mounted to  
a ball screw nut 67 which converts rotation of ball  
15 screw 66 into linear translation of plunger drive  
ram 62 into or out of power head 22, thus moving the  
plunger 37 (Fig. 2) of a syringe 36 mounted to power  
head 22. Knob 49 is coupled to the axis of drive  
pinion 64, thus permitting hand rotation of the  
20 drive train 60 and motion of the plunger drive ram.

These elements of the drive train 60 are  
mounted to a drive housing 69. When the upper and  
lower half-housings 47a and 47b are assembled around

the drive housing 69, the front surface 70 of drive housing 69 is exposed. The face plate 28 of the injector is attached to front surface 70, to allow a syringe to be mounted to the front surface 70 of the drive housing 69 so that plunger drive ram 62 may engage and move the syringe plunger 37.

The face plate 28 is attached to front surface 70 by a hinged connection, using a hinge pin 72. When face plate 28 has been attached to front surface 70 with hinge pin 72, face plate 28 may rotate in direction 73 on hinge pin 72, and may also translate in direction 74 over a limited distance along hinge pin. This combination of rotational and translational movement allows face plate 28 to be engaged and disengaged from front surface 70, permitting loading and removal of syringes from face plate 28, and simultaneous coupling and uncoupling of the syringe plunger from plunger drive ram 62.

When face plate 28 is fully engaged to front surface 70, tabs 75a and 75b on face plate 28 mate to slots 76a and 76b, respectively, on front surface 70. This mating relation is shown in greatest detail in Fig. 4. To disengage face plate

28 from front surface 70, face plate 28 is translated along direction 74 to disconnect tabs 75a and 75b from slots 76a and 76b, permitting face plate 28 to rotate on hinge pin 72 in direction 73 (Fig. 3), thus permitting access to a syringe mounted to face plate 28.

To facilitate translation of face plate 28 along direction 74, a cam lever 78 is mounted to drive housing 69 between face plate 28 and drive housing 69. Cam lever 78 is affixed to and rotates a cam lever shaft 79, which is mounted in drive housing 69. Cam lever 78 includes a button 81 which projects toward face plate 28. Button 81 mates with a channel 80 formed in the inner surface of face plate 28 (see Fig. 4), so that rotation of cam lever 78 causes button 81 to translate face plate 28 along direction 74, engaging or disengaging tabs 75a and 75b from slots 76a and 76b.

A flag washer 82 is mounted to cam lever shaft 79 and held in place with a nut 83. The apertures in flag washer 82 and cam lever 78 which connect to cam lever shaft 79 are keyed, so that cam lever 78 and flag washer 82 are oriented in a

consistent manner relative to each other. Because  
flag washer 82 and cam lever 78 are both keyed to  
shaft 79, rotation of cam lever 78 will cause shaft  
79 and flag washer 82 to rotate. Flag surface 84  
5 extends from flag washer 82; movement of this flag  
surface due to rotation of cam lever 78 is detected  
as noted below and used to determine whether face  
plate 28 is engaged to the power head 22.

Referring now to Figs. 3 and 4, when power  
10 head 22 is assembled as shown in Fig. 4, flag washer  
82 is positioned opposite to flag sensor 58 on  
circuit board 55. Flag sensor 58 produces a light  
beam which, when flag surface 84 is opposite to  
sensor 58, will be reflected and detected by sensor  
15 58. Cam lever 78 and flag washer 82 are keyed into  
shaft 79 so that flag surface 84 is rotated opposite  
to detector 58 only when cam lever 78 is positioned  
as shown in Fig. 4, in which position cam lever 78  
will have translated cam face plate 28 into  
20 engagement with the front face 70 of drive housing  
69, permitting injection. Thus, when flag surface  
84 is opposite to flag sensor 58, this indicates

that the face plate is in the closed position, ready for filling or injection.

Power head 22 includes a safety lock-out which prevents rotation of cam lever 78 to a  
5 disengaged position when plunger drive ram 62 is other than fully retracted. Specifically, referring to Fig. 4, a spring loaded lockout plate 86 is mounted to drive housing 69 in a manner to permit translational movement in direction 90. Screws 87  
10 hold lockout plate 86 in position on drive housing 69 to allow this translational movement. Spring 88 is coupled between lockout plate 86 and drive housing 69 to provide force tending to slide lockout plate 86 toward front surface 70 of drive housing  
15 69, i.e., into the position shown in Fig. 4.

When lockout plate 86 is in this forward most position, the front corner 89 of lockout plate 86 is positioned adjacent to flag washer 82, as seen in Fig. 4. As a result, interference between a  
20 notch 85 (see Fig. 3) in flag washer 82 and front corner 89 of lockout plate 86 prevents rotation of flag washer 82 (and cam lever 78) from the engaged position shown in Fig. 4 to a position where face

plate 28 will disengage from front surface 70 of  
drive housing 69, and can be rotated away from front  
surface 70 to replace a syringe. However, when  
lockout plate slides backward in direction 90  
5 (against the force of spring 88), this interference  
between front corner 89 and notch 85 in flag washer  
82 is eliminated, allowing cam lever 78 to rotate to  
a disengaged position.

65071"044660  
10 A fitting 91 on plunger drive ram 62 is  
positioned to engage to lockout plate 86, so that  
when plunger drive ram 61 is withdrawn from the face  
plate 28 to a fully rearward position, fitting 91  
will engage lockout plate 86 and move it to its  
backward position. However, when plunger drive ram  
15 62 is moved forward from this position, the force of  
spring 88 moves lockout plate into its forward  
position. Thus, as a result of the interaction of  
plunger drive ram 62, lockout plate 86 and flag  
washer 82, face plate 28 cannot be translated in  
20 direction 74 or disengaged from front surface 70 of  
drive housing 69 unless the plunger drive ram 62 is  
at its fully rearward position. This interlock  
prevents the operator from attempting to disengage

face plate 28 from front surface 70 while plunger drive ram 62 is projecting inside of a syringe mounted to face plate 28.

Referring now to Figs. 4 and 5, there is illustrated three magnetic conductors 94a, 94b and 94c. These conductors are manufactured of a high permeability, low retentivity material such as steel or iron, and are inserted through apertures in the front surface 70 of drive housing 69.

Each face plate 20 may be provided with permanent magnets inserted at positions which are in registration with the positions of the three magnetic conductors 94a, 94b and 94c. There may be three, two, one or no permanent magnets, and the magnets may be oriented with their North or South poles facing magnetic conductors 94a, 94b and 94c.

The face plate 28 shown in Fig. 4 includes two permanent magnets 96a and 96b positioned in registration with magnetic conductors 94a and 94b. The face plate shown in Fig. 4 does not, however, have a magnet positioned opposite to magnetic conductor 94c.

Multiple different face plates 28 may be used with the power head 22 illustrated in Figs. 3 and 4. Different face plates 28 may be used to adapt the power head 22 to use different types of syringe 36; for example, one face plate may be sized for use with low capacity pediatric syringes, whereas another is sized for use with adult-capacity syringes. Pre-filled syringes may have different sizes or dimensions than syringes which are purchased empty. Different face plates 28 are needed to accommodate these different syringe sizes.

It is necessary for the control circuitry on circuit board 55 to be able to detect which face plate is installed on power head 22. Firstly, the control circuitry must determine whether an air detection module is attached to the face plate. Also, different syringe 36 types may have differing lengths, in which case power head 22 must be able to compensate for the length variations when determining the end-of-travel position of the plunger drive ram and when computing the volume of fluid in the syringe 36. Similarly, syringes of different diameters will produce different flow

rates for the same rate of travel of the plunger drive ram 62; the control circuitry must compensate for this when converting a requested flow rate into movement of the plunger drive ram 62.

5                   For identification purposes, each different face plate 28 has a unique combination of permanent magnets installed therein, in registration with the magnetic conductors 94a, 94b and 94c in the front surface 70 of the drive housing 69.

10                   Specifically, the face plate illustrated in Fig. 4 has two permanent magnets, opposite conductors 94a and 94b. Another face plate might have only one permanent magnet, positioned opposite conductor 94b. A third face plate might have three permanent

15                   magnets positioned opposite all three conductors 94a, 94b and 94c. There are twenty-seven ( $3^3$ ) possible combinations of magnets, or the lack thereof, at alternative polarities, that can be created, and thus twenty-seven different face plates

20                   can be uniquely identified in this manner.

                  To detect the number and positioning of permanent magnets in the face plate, the control circuit of the power head 22 includes magnetic

660701  
5 detectors 56a, 56b and 56c, which may for example be  
Hall effect sensors (or, alternatively, reed  
switches). These three magnetic detectors 56a, 56b  
and 56c are positioned near an edge of circuit board  
55 in registration with the inner ends of the three  
magnetic conductors 94, as can be seen by comparing  
Figs. 4 and 5. Typically, the drive housing 69 is  
manufactured of a non-magnetic material such as  
Aluminum. Accordingly, magnetic fields produced by  
10 permanent magnets 96a and 96b are channeled through  
the magnetically permeable conductors 94a, 94b and  
94c, and thus brought into the vicinity of detectors  
56a, 56b and 56c, so that the presence or absence of  
permanent magnets in face plate 28 can be detected  
15 remotely from the face plate 28 by detectors on  
circuit board 55.

The magnetic conductors, by channeling  
magnetic fields from permanent magnets in the face  
plate 28 to remotely located detectors on circuit  
20 board 55, provide a substantial reduction in cost of  
the electronic portion of the power head 22.  
Although free-standing magnetic detectors are  
available, and could be mounted to the front surface

70 of drive housing 69, free-standing magnetic detectors are typically substantially more expensive to purchase than printed circuit board mountable detectors. Furthermore, the use of free-standing magnetic detectors would entail manufacturing multiple separate circuit boards and/or harnesses and installing them in the power head housing with appropriate cabling connections to the main circuit board, which would make the manufacture of power head 22 more complex, expensive and time-consuming, as compared the present embodiment where the detectors are included on the main circuit board. Accordingly, the use of magnetic conductors 94a, 94b and 94c substantially reduces the cost of manufacturing power head 22.

Referring to Fig. 6, the details of the hand-operated movement control can be explained. As noted above, hand-operated control lever 29 is rotated in a forward direction or reverse direction to indicate the operator's desire to move the plunger drive ram forward or in reverse. To determine the direction and degree of rotation of lever 29, a rotary potentiometer 98 is coupled to

shaft 48 of lever 29, so that rotation of lever 29 rotates a wiper inside of potentiometer 98, creating a changing resistance that can be detected by the power head control circuitry.

5                   As noted above, when control lever 29 is rotated forward in direction 99, the control circuitry, detecting this rotation from electrical signals produced by potentiometer 98, causes the plunger drive ram 62 to move forward, i.e., outward  
10                   from the power head housing, at a velocity proportional to the angle of deflection of control lever 29 away from the home position shown in Fig. 6. Alternatively, when control lever is rotated in a reverse direction 100, the control circuitry  
15                   detects this rotation from electrical signals produced by potentiometer 98, and causes the plunger drive ram 62 to move backward, i.e., into the power head housing, at a velocity proportional to the angle of deflection of control lever 29 away from  
20                   the home position shown in Fig. 6.

Fig. 6 illustrates the two return springs 102a and 102b which engage shaft 48 and produce torque tending to return shaft 48 to the home

position shown in Fig. 6. Also shown is the  
combined flag/contact 104 which surrounds shaft 48  
and contacts return springs 102a and 102b. Return  
springs 102a and 102b make contact with flag/contact  
5 104 and thereby form an electrical connection to  
each other, and also apply spring torque tending to  
return shaft 48 to the home position. Also seen are  
detent spring 106, the function of which will be  
elaborated below, and flag detector 108, which is an  
10 optical detector which generates a light pulse for  
transmission across a gap, detects receipt of the  
light pulse on the opposite side of this gap, and  
generates a digital signal indicative of whether the  
gap is obstructed in such a way as to prevent light  
15 transmission.

Referring now to Figs. 6, 7A and 7B, it  
can be seen that when lever 29 is in its home  
position (see Figs. 6 and 7A), flag/contact 104 is  
positioned equidistant between return springs 102a  
20 and 102b, which apply opposing torques to lever 29,  
tending to hold lever 29 in this home position. In  
this position, flag 105 of combined flag/contact 104  
is positioned inside of flag sensor 108, causing

sensor 108 to produce a digital signal indicating  
that the lever is in its home position. In this  
case, the control circuit of power head 22 can  
determine that no plunger motion is being requested  
5 through the hand-operated movement control.

However, when lever 29 is rotated from its  
home position, such as in Fig. 7B, flag 105 moves  
outside of the gap formed by flag sensor 108,  
causing flag sensor 108 to produce a digital signal  
10 indicating that lever 29 is away from the home  
position. In this case, the control circuit may  
read the electrical signal produced by potentiometer  
98 to determine the position of the lever and  
produce the appropriate motion of the plunger drive  
15 ram.

As noted above, the velocity of motion of  
the plunger drive is proportional to the extent of  
rotation of lever 29 away from its home position.  
At the same time, the mechanical structure of return  
20 springs 102a and 102b ensures that a return torque  
is applied to lever 29 as lever 29 is rotated to  
increasing angles away from the home position.  
Depending on the stiffness of springs 102a and 102b,

and the range of motion of lever 29, this return torque may be approximately equal at all deflection angles, or may increase or decrease over increasing deflection angles. An increasing return torque with  
5 deflection angle, may be useful in providing the operator with additional feedback on the plunger velocity.

As can be seen in Fig. 7B, as lever 29 is rotated to increasing angles in the reverse  
10 direction, ultimately flag 105 contacts detent spring 106 and begins deflecting detent spring 106 as well as return springs 102a and 102b. This leads to an increase in applied torque that is detectable to the operator, as a "detent" in the rotation of  
15 the hand-operated movement control.

When filling a syringe, there is an ideal maximum speed at which fluid can be drawn into the syringe without forming air bubbles in the fluid due to non-laminar flows. To speed the filling of  
20 syringes, the operator should have feedback as to when this ideal speed has been reached, so that syringes can be filled at this optimal speed. The purpose of the detent spring 106, is to provide the

operator with mechanical feedback of the angle of  
deflection of lever 29 which corresponds  
approximately to the ideal fill speed. More  
specifically, the control circuit of power head 22  
5 establishes that the plunger drive will move at near  
to the ideal fill speed when lever 29 has been  
rotated such that flag 105 is in contact with detent  
spring 106. Accordingly, an operator wishing to  
fill a syringe at a near ideal speed, can rotate  
10 lever 29 until the increasing torque of the detent  
is noted, and then hold lever 29 at the detent  
location to fill the syringe.

The return springs 102, flag/contact 104  
and return spring 106 are not only mechanically  
15 active to provide mechanical feedback to the  
operator, but are also electrical elements in the  
control circuit of power head 22. Specifically,  
referring to Fig. 7C, each of these elements is an  
electrical circuit element in a circuit for  
20 producing digital control signals used by the  
control of power head 22.

As seen in Fig. 7C, return springs 102a  
and 102b, and the flag/contact therebetween, are

connected with a resistor 110 in a series connection  
between a digital +5 volt power supply and ground.  
A signal line 115 extending from between resistor  
110 and spring 102a carries a logic voltage signal  
5 indicating whether a current-carrying electrical  
contact is completed between springs 102a and 102b  
and flag/contact 104. Under normal conditions,  
there should be an electrical path through this path  
to ground, holding the voltage on line 115 at a low  
10 level, indicating proper operation. However, if one  
of springs 102a or 102b fails, and no longer engages  
flag/contact 104, this electrical contact will be  
broken, and the voltage on line 115 will be elevated  
to a high level, indicating failure of a return  
15 spring. Although both return springs must fail  
before lever 29 may unintentionally deflect away  
from the home position, failure of just one spring  
can be detected by monitoring the voltage on line  
115. Upon initial detection of such a failure, a  
20 warning may be given to the operator, or  
alternatively, the hand-operated movement control  
may disabled.

66011" 0744660

In a similar fashion, the detent spring 106 forms an electrical contact in a series connection with a resistor 111, and a detent signal line 116 extends from between resistor 111 and the detent spring. If control lever 29 is not rotated into the detent spring, line 116 will be pulled to a high level, indicating that the control lever 29 is not at the detent. However, if control lever 29 is rotated such that flag 105 contacts detent spring 106, line 116 will be pulled to a low level, indicating that control lever 29 has been rotated to the detent. The signal on line 116 may be used in several ways. For example, the signal may be used to calibrate the hand-operated control so that the angle of lever rotation corresponding to the detent is equal to the ideal fill speed. Alternatively, the signal may be used to prevent reverse movement of the ram at a speed faster than the ideal fill speed. Finally, the signal may be used to establish a "dead zone" of motion, in which the ram will move at the ideal fill speed, while permitting the lever to be rotated beyond the "dead zone" to produce faster reverse speeds.

Fig. 7C also illustrates the circuit details of the flag detector 108; a light emitting diode is energized with a bias current via resistor 113; when light passes through the gap in detector 108 and strikes the base of a phototransistor in detector 108, the phototransistor draws current through resistor 112 to drive a home signal on line 117 to a low value, indicating that control lever 29 is not in its home position. Otherwise, if light is unable to pass to the base of the phototransistor in detector 108, current is not drawn through resistor 112 and the home signal on line 117 is pulled to a high value, indicating that control lever 29 is in its home position. The control circuitry for power head 22 can thus use the home signal on line 117 to determine whether to discontinue motion of the plunger drive ram.

Referring now to Fig. 8, the heater blanket 42 used with the power head 22 in accordance with the present invention, includes an annular plastic section 118 and a molded plastic base. Plastic section 118 includes a filament 120 of electrically resistive wire, which generates heat

when an electrical current is driven through it via  
a suitable electrical power source. Filament 120  
extends throughout the region of annular section 118  
which is in contact with pressure jacket 38 when  
5 heater blanket 42 is mounted to post 44 as shown in  
Fig. 2, and terminates at either end in electrical  
leads encased in an insulating cable 117 which can  
be plugged into the power head 22 control circuitry  
through aperture 51 (Fig. 3) as is illustrated in  
10 Fig. 2. When current from the power head is forced  
through the leads in cable 117 and through the  
filament 120, filament 120 generates an even heat  
which warms fluid inside of the syringe in pressure  
jacket 38.

15           Annular section 118 might be opaque, or  
may be clear or translucent. If annular section 118  
is clear, filament 120 could be seen through (as in  
an automobile defroster or a window screen) so that  
the operator is better able to visualize fluid  
20 inside of the syringe through the annular section,  
pressure jacket 38 and syringe wall. This may be  
advantageous in applications where the operator's

primary line of sight to the interior of the syringe might otherwise be obscured by the heater blanket.

Base 119 of heater blanket is formed of a soft plastic, overmolded on a resilient skeleton.

5 The resilient skeleton is shaped with a bowl 121 sized for a slight interference fit with post 44. As a result, heater blanket 42 may be snap fit over post 44 for convenient installation and removal (e.g., for cleaning).

10 Referring now to Figs. 9 and 10, the integral air detection system can be described. The air detection module 122 is mounted to the end of post 44, and is configured to wrap around the distal end of pressure jacket 38 and into contact with an  
15 outwardly projecting collar 124a surrounding the discharge neck of syringe 36. At the point of contact with collar 124a, the air detection module includes a light source 126 and light sensor 127. Light sensor 127 is a commercially available  
20 circuit, which includes sensor 127 and an oscillator which produces a trigger signal indicating when light source 126 should be stimulated to produce a light beam. The output of sensor 127 is a digital

signal indicating whether the light beam is received by detector in response to triggering of the light source.

5 Figs. 9 and 10 show illustrative ray traces showing the paths taken by light rays emitted from light source 126. Light source 126 includes an integral focusing lens, and collar 124a on the discharge neck of syringe 36 forms a second focussing lens. These lenses act in concert to  
10 direct light from light source 126 along path 129 toward collar 124b on the discharge neck of syringe 36. The internal shape of collar 124b forms a corner reflector, so that light impingent upon collar 124b from light source 126 is reflected  
15 toward light sensor 127.

As a result of this structure, when the neck of syringe 36 is filled with fluid, light rays emitted from light source 126 follow paths through the neck of syringe 36, which reflect and return to  
20 light sensor 127, such as path 129 illustrated in Figs. 9 and 10. Accordingly, under such conditions, sensor 127 will produce a digital signal indicating receipt of light, which indicates the absence of air

in the syringe neck. (The combined focal length of the lens in light source 126 and collar 124a, is longer than the distance travelled by light along path 129, i.e., longer than twice the distance between collar 124a and collar 124b.)

However, when the neck of the syringe contains air or an air bubble, diffraction of light at air/fluid or air/syringe boundaries will cause light to deviate substantially from the path 129 illustrated in Figs. 9 and 10. Specifically, light rays incident in the neck of syringe 36 might follow the path 130 illustrated in Fig. 9, or the path 131 illustrated in Fig. 10. In either circumstance, the presence of the air bubble prevents light from reflecting through the neck of the syringe from light source 126 to light detector 127, thus causing the light detector to produce a signal indicating failure to receive light, indicating that air is present in the neck of the syringe.

To ensure consistent, repeatable results, air detection module 122 is structured to ensure solid contact between light source 126, light sensor 127 and the surface of collar 124a on syringe 36.

Specifically, the air detection module 122 has a  
spring-metal interior skeleton 133, which is  
overmolded with a soft flexible plastic 134. One  
end of spring metal skeleton 133 is mounted to post  
5 44 by mounting screws 135 (which are accessible via  
voids in the plastic overmold 134). The opposite  
end of skeleton 133 supports the air detector  
module, which includes a hard plastic molding 136  
supporting the light source 126 and light sensor  
10 127. Molding 136 includes a beveled section 137  
sized to fit into a chamfer 138 at the aperture of  
pressure jacket 38. The interaction of beveled  
section 137 and chamfer 138 ensure precise  
positioning of light source 126 and light sensor 127  
15 relative to pressure jacket 38.

The neck of the syringe 36 is sized with a  
slight interference fit, so that collar 124a  
contacts and slightly deflects air detection module  
122 when the syringe 36 is inserted into pressure  
20 jacket 38, flexing spring skeleton 133 and resulting  
in a steady application force of light source 126  
and light sensor 127 against collar 124a of syringe  
36. This application force ensures good

communication of light from source 126 into the neck  
of syringe 36 and from the neck of syringe 36 into  
light sensor 127.

Now turning to Fig. 11A, the electrical  
5 circuit details of the air detection module, and  
other analog electrical systems, can be elaborated.  
Specifically, the air detection module incorporates  
therein, a commercially available synchronous  
detection circuit 140, which includes an internal  
10 oscillator generating trigger pulses on line 141,  
and, contemporaneously with each trigger pulse,  
detects electrical signals on line 142 indicating  
that light has been received at light sensor 127.  
So long as light is detected contemporaneously with  
15 each trigger pulse, a high level signal is produced  
on line 143. Due to the application to which  
circuit 140 is applied in accordance with the  
invention, the signal on line 143 indicates whether  
air has been detected in the neck of the syringe 36.

20 The control circuit of power head 22 may  
control the light intensity applied to the air  
bubble detector, to control the sensitivity of the  
detector. To do so, the control circuit produces a

pulse width modulated (PWM) digital signal on line  
145. This PWM signal is filtered by a low-pass  
filter circuit 146 to produce an analog control  
voltage, which controls an adjustable regulator 147  
5 to produce the power signal on line 148 for circuit  
140.

In response to the trigger signal on line  
141, a PNP opto-transistor 149 is turned "on",  
causing the power signal on line 148 to energize  
10 light source 126. Thus, the voltage of the power  
signal on line 148 directly affects the intensity of  
light generated by light source 126.

So that the control circuit may monitor  
the air detector circuit 140 for possible failures,  
15 the trigger signal on line 141 is connected to the  
base of PNP opto-transistor 149 via a light emitting  
diode in an opto-isolator 150. Accordingly, the  
opto-transistor in opto-isolator 150 will turn "on"  
whenever the trigger signal is activated, causing a  
20 "low" level to appear on line 151. Thus, if the  
synchronous air detector circuit 140 is operating  
properly and producing periodic trigger signals,  
pulses will appear on line 151, which can be

detected by the control circuit to verify that the oscillator in circuit 140 is operating properly.

Fig. 11A also illustrates the analog-to-digital (A/D) converter 152 incorporated into the power head control circuit for quantizing analog signals produced by various electrical elements. For example, potentiometer 98 (see Fig. 6) is connected to the shaft 48 of fill/expel lever 29. The wiper of this potentiometer is connected to a signal line 154, which carries an analog voltage indicative of the rotational position of the fill/expel lever shaft 48. The opposite ends of the potentiometer are connected to a reference voltage and to ground, so that the voltage on line 154 lies somewhere between these extremes, dependent upon the rotational position of fill/expel lever 29. Line 154 connects to A/D converter 152, and converter 152 converts the analog voltage on line 154 to a digital signal on a "SPI" serial interface bus 156, upon request from the CPU (see Fig. 11B), so that the CPU can determine the position of fill/expel lever 29 and react accordingly.

Other analog voltages are also input to A/D converter 152. Specifically, a single-chip accelerometer is configured as a tilt sensor 158, to produce an analog voltage on line 159 indicative of the angle of tilt of sensor 158. (A suitable single chip accelerometer for this purpose is available from Analog Devices of Norwood, Massachusetts as part no. ADXL05AH.) Sensor 158 is mounted to circuit board 55, and therefore produces an output voltage indicative of the tilt of power head 22 relative to the direction of Earth gravity. This analog tilt signal is converted and input to the CPU for use, as noted below, in controlling the display and other operational features of power head 22.

A third analog signal is produced by a linear potentiometer 160, the wiper of which is mechanically connected to the plunger drive ram 62, and moved in response to movement of the plunger drive ram. Thus, the voltage of the wiper on line 161 is an analog signal representative of the position of the ram between its rearward most and forward most positions. This signal is converted and used by the CPU to determine the position of the

ram and, among other things, the syringe volume remaining.

Two additional analog signals are produced by thermistors 163A and 163b, which are series  
5 connected with bias resistors to produce voltages on lines 164a and 164b which reflect the temperature of the thermistors. The temperature measurement obtained from these thermistors is then used to control the power applied through the heater blanket  
10 to warm the fluid in the syringe 36. Specifically, the heat power applied to the syringe is varied proportion to the ambient temperature, as measured by thermistors 163a and 164a, to maintain the fluid at the target temperature, e.g., 30 degrees Celsius.

15 Thermistors 163a and 163b are duplicative, that is, both measure the same temperature and their measurements are compared to ensure near agreement. As a result, failure of a thermistor can be detected from disagreement between the temperature readings  
20 obtained from the thermistors, preventing loss of temperature control.

Thermistors 163a and 163b may be mounted internally to power head 22, on circuit board 55.

Alternatively, thermistors 163a and 163b may be external to the housing, to ensure more accurate temperature readings, or both options may be allowed by providing internally-mounted thermistors which  
5 can be disabled if substitute externally-mounted thermistors are connected to the power head 22.

As noted above, using thermistors 163a and 163b, power head 22 controls the heat power applied to the syringe 36 through heater blanket 42. To  
10 perform this function, the CPU (see Fig. 11B) produces a pulse width modulated (PWM) control signal on line 166 which is used to control the heat power applied to the heater blanket filament 120. Specifically, the PWM signal on line 166 is low pass  
15 filtered by filter 167, producing an analog control signal which controls an adjustable regulator 168. The output of regulator 168 on line 169 is a variable voltage which is applied across heater blanket filament 120, causing heater filament 120 to  
20 produce heat.

An instrumentation amplifier 170 filters and conditions the voltage across filament 120 to produce an analog output signal on line 171 which is

proportional to the voltage applied to the heater  
blanket filament 120.

A sense resistor 173 is series connected  
with heater filament 120, so that the current in  
5 heater filament 120 passes through sense resistor  
173, producing a voltage on sense resistor  
proportional to the current flowing through heater  
filament 120. Sense resistor has a resistance  
substantially smaller than that of heater filament  
10 120, so that the small voltage drop across sense  
resistor 173 is not a substantial percentage of the  
voltage drop across heater filament 120.

The voltage drop across sense resistor 173  
is amplified and filtered by a gain/filter circuit  
15 172, producing an analog voltage on line 174 which  
is proportional to the current flowing through  
heater filament 120.

Lines 171 and 174 are connected to A/D  
converter 152, and the voltages on lines 171 and 174  
20 are converted thereby to digital signals which can  
be read by the CPU. Accordingly, the CPU can  
determine the current and voltage drop across heater  
filament 120, and use these values to determine the

heat output of heater filament 120. This permits the CPU to perform closed-loop control of the heater blanket heat output, as discussed below in connection Fig. 12.

5                   Referring now to Fig. 11B, the connections to the CPU of the power head 22 can be understood. The CPU 175, which may be a 68332 microprocessor, available from Motorola, controls data and address busses 176 connecting CPU 175 to random access  
10                   memory (RAM) 178 and a flash memory 177. CPU 175 also controls an SPI serial interface bus 156 for communicating with A/D converter 152, display 30 and a monitor microcontroller 192. CPU 175 further includes an RS-422 serial interface 179 connecting  
15                   CPU 175 to a CPU in the power pack (see Fig. 11C).

                  CPU 175 includes a number of digital data input lines for monitoring operation of power head 22. Specifically, CPU 175 receives the detent  
20                   signal on line 116, safe signal on line 115 and home signal on line 117, enabling CPU to receive input on the state of operation of the hand-operated movement lever as discussed above. CPU 175 also receives the bubble signal on line 143 from which CPU 175 may

detect air in the syringe neck and take appropriate  
action, and in addition, CPU 175 receives the bubble  
detection oscillator signal on line 151, which can  
be used as noted above to confirm proper operation  
5 of the oscillator in the air detection module 122.  
Further, CPU 175 receives the output of flag sensor  
58, from which CPU 175 may determine whether the  
face plate is securely locked to the housing of  
power head 22. Furthermore, CPU 175 receives  
10 digital signals from the three magnetic detectors  
56a, 56b and 56c indicative of which of several  
possible face plates are mounted to power head 22,  
allowing CPU 175 to adjust its operation  
accordingly.

15 CPU 175 also receives digital input  
signals from parallel rotary encoders 182, which  
produce pulse signals on lines 183a and 183b  
indicative of rotation of the plunger drive train.  
These pulses are used by CPU 175 to confirm movement  
20 of the plunger drive ram. Lines 183a and 183b are  
also connected to the power pack (see Fig. 11C) so  
that the power pack CPU may perform closed loop  
control of plunger movement by counting encoder

pulses and comparing the rate of receipt of encoder pulses to a desired rate. A closed loop control is disclosed in U.S. Patent No. 4,812,724, which is incorporated by reference herein in its entirety.

5 CPU 175 also produces multiple digital control signals, including those noted above, i.e., the air bubble detector power PWM signal on line 145, and the heater blanket power PWM signal on line 166, both being pulse-width modulated by CPU 175 to produce desired power levels. CPU 175 further produces output signals on lines 187 for illuminating light emitting diodes in lamp 46 (Fig. 2) which indicate the status of operation of the injector. Additional output signals on SPI serial bus lines 156 control the display 30.

15 CPU 175 uses the above-noted inputs and outputs to perform primary control of power head 22 under control of software resident in CPU 175 or read from RAM 178. As noted above, CPU 175 is also connected, through SPI serial bus 156, to a microcontroller 192 which serves as a monitor, for monitoring operation of CPU 175 to ensure the absence of software or hardware failures.

(Microcontroller may be a single-chip microcontroller available from Microchip Technologies as part no. PIC16C63.) Monitor microcontroller 192 performs this function by  
5 receiving, through bus 156, an indication of the current operational state of CPU 175.

Specifically, CPU 175 indicates, through bus 156, the operating state of CPU 175, i.e., whether CPU 175 is requesting movement of the  
10 plunger or not, and whether the motion is being requested in response to hand-operated or automatic (programmed) control, and potentially other specific information such as the rate of movement that is being requested. Monitor microcontroller 192 reads  
15 this state information from lines 156, and compares this information to crucial digital input signals from the power head 22, to ensure consistency therebetween.

For example, microcontroller 192 receives  
20 the safe signal on line 115 and home signal on line 117. If these signals indicate that the hand-operated control is in the home position, then CPU 175 should not be generating movement under hand-

operated control. If a spring has failed (as indicated by the signal on line 115), this should be reflected in the state of the CPU 175. Therefore, under these conditions, microcontroller 192 reads the state information from bus 156 to ensure that CPU 175 is not acting inconsistently with the signals from the hand-operated control.

As a second example, microcontroller 192 receives the output signals from rotary encoders 182 on lines 183a and 183b. Microcontroller 192 checks these signals to determine whether the plunger drive ram is moving, to ensure the drive ram is moving only when the state of CPU 175 indicates that the drive ram should be moving, and not otherwise.

Furthermore, in this connection it should be noted that microcontroller 192 receives the door flag signal from door flag sensor 58. If this signal indicates that the door of power head 22 is other than in the locked position, CPU 175 should not be requesting movement of the plunger drive ram, and microcontroller 192 confirms this by checking for the absence of pulses from encoders 182.

Referring now to Fig. 11C, the interaction of the power head 22, power pack 26 and console 24 can be further understood. Specifically, each of power head 22, power pack 26 and console 24 contains a CPU 175, 192 and 194, respectively. These CPUs interact through external interfaces to perform control of the injector. For example, the plunger drive ram can be controlled through the lever 29 on power head 22 (as discussed above), or can be automatically controlled by an operator entering programs for injections using touch screen 32 of console 24 (using CPU 194), and then enabling the programmed injection. The injection parameters such as motor speed and injection volumes will then be produced by console CPU 194, which communicates with power pack CPU 192 to cause these programmed actions to take place. Furthermore, an automatic injection may be enabled using the touch screen 32, or an injection may be started using a hand switch or OEM remote trigger connected to power pack 26. In either case, the appropriate one of CPUs 192 and 194 generates an enabling signal to initiate the automatic injection.

As noted above, the power head CPU 175 is associated with a monitor microcontroller 192 for monitoring the state of CPU 175 to ensure its actions are consistent with input signals from power head 22. Similarly, CPUs 192 and 194 are also associated with monitor microcontrollers 196 and 198, respectively, which monitor the actions of the associated CPUs 196 and 198 to ensure consistent, error free behavior.

Monitor microcontrollers 192, 196 and 198 communicate with each other in a manner which parallels the communication of CPUs 175, 192 and 194. Specifically, the three monitor microcontrollers exchange state information received from their associated CPUs to ensure that the three CPUs are in similar states of operation, e.g., hand-operated movement, automatic movement, no movement, etc. Furthermore, each of the microcontrollers receives external input signals to ensure that state transitions which should occur are, in fact, occurring. Thus, microcontroller 196 receives the hand or OEM trigger signals so that microcontroller 196 can determine when an automatic injection has

been triggered. Microcontroller 198 receives input signals from touch screen 32 so it, too, can determine when an automatic injection has been triggered. Other monitoring functions can be performed, as desired to ensure correct and consistent operation of CPUs 175, 192 and 194.

As noted above, power head CPU 175 delivers a control signal to power pack 26, requesting a ram movement. Power pack 26 contains the motor servo control circuitry for producing an appropriate power signal on line 200 to drive motor 63, and to perform closed loop control of motor movements in response to encoder pulses on lines 183.

In error conditions, the monitor microcontrollers can discontinue power flow to motor 63 through a hardware disable, represented by switch 202 in series with power line 200, thereby ceasing any movement of the plunger drive. This hardware disable ensures that the monitor microcontrollers can prevent erroneous injection of fluid under error conditions.

Referring now to Fig. 12, the heater blanket control functions performed in power head CPU 175 may be explained. To perform heater blanket control, CPU 175 initially measures the ambient temperature using the first and second thermistors 163a and 163b (steps 204 and 206). (As part of these steps, CPU 175 may reference stored compensation tables for converting thermistor voltages to corresponding temperatures.) CPU 175 then determines whether these temperature readings are consistent with each other (step 208). If not, this indicates a fault in a thermistor, and an alarm is generated, and the heater blanket is disabled (step 210).

15            If the thermistor temperature readings are similar, then CPU 175 proceeds to determine a desired heater blanket power output level  $P_{OUT}$  (step 210), based on the measured ambient temperature  $T_{AMBIENT}$ . A thermal model is used to calculate the power required to maintain the fluid temperature at 37° C with the measured ambient temperature. The power will vary according to this model over the range of ambient temperatures from 0° C to 32° C. Above an ambient temperature of 32° C, the heater

blanket is shut off to avoid over heating the fluid.  
Below an ambient temperature of 0° C, the power  
produced by the heater blanket is limited to 8 Watts  
to avoid overheating the heater filament 120 in the  
5 heater blanket. One simplified thermal model would  
be a linear model, in which the output power is  
determined by the formula  $P_{OUT}=B-AT_{AMBIENT}$ , where B and  
A are empirically computed offset and gain factors,  
and  $P_{OUT}$  is limited to eight Watts. Other models  
10 might also be used, particularly non-linear models.

To produce this desired output heat power,  
CPU 175 produces a PWM signal on line 166 (Figs. 11A  
and 11B) at a duty cycle (step 212). An initial  
duty cycle is chosen to begin warming the fluid in  
15 the syringe.

As this PWM duty cycle is produced, CPU  
175 reads, from lines 171 and 174 (through A/D  
converter 152), the analog voltages indicating the  
voltage and current applied to heater filament 120  
20 (steps 214 and 216). These values are multiplied to  
determine the actual power being output from the  
heater blanket, and this power is compared (step  
218) to the desired output power computed earlier.  
If the current output power is approximately equal

to the desired power, then the current PWM duty  
 cycle is correct, and CPU 175 will return to step  
 204 to re-measure the ambient temperature to  
 continue controlling the heater output power. If,  
 5 however, the heater output power is either too large  
 or too small, CPU 175 will proceed first to step  
 220, and adjust the PWM duty cycle to change the  
 heater output power as needed (by reducing the duty  
 cycle if too much power is being produced, or by  
 10 increasing the duty cycle if too little power is  
 being produced). Thereafter, CPU 175 will return to  
 step 204 to re-measure ambient temperature to  
 continue controlling the heater output power.

This temperature control methodology  
 15 ensures accurate control of the temperature of the  
 fluid in syringe 36, compensating for temperature  
 variations which can be caused by variations in  
 ambient temperature, thus reducing the likelihood of  
 thermal shock in the subject caused by injection of  
 20 fluid which is not at the desired temperature.

Now referring to Figs. 13A-13C, the  
 operation of the invertible display can be  
 understood. Specifically, as noted above, CPU 175  
 receives a signal from tilt sensor 158 indicative of

the angle of power head 22 relative to Earth gravity. CPU 175 repeatedly samples this signal, and determines the angle of power head 22 with respect Earth gravity (direction 222). All possible  
5 angles of rotation are divided into six regions of operation, illustrated in Fig. 13A.

Region 1 is the "fill" region; it is the angle at which the power head 22 should be placed for filling the syringe. When the power head 22 is  
10 at an angle within region 1, or within regions 2a or 2b which are adjacent thereto, the power head will permit hand-operated motion of the plunger drive ram in either the forward or reverse direction, allowing the operator to fill the syringe and remove air from  
15 the syringe after initial filling. A wide range of movement speeds can be generated with the hand-operated movement control, permitting rapid filling of the syringe. While the power head 22 is in regions 1, 2a or 2b, however, programmed injections  
20 are inhibited; thus, the operator cannot initiate injection of a subject according to a pre-programmed injection protocol while the power head 22 is in an upright position. This minimizes the likelihood of accidental injection of air into the subject.

Region 4 is the "inject" region. When the power head 22 is tilted in this region, programmed injections can be initiated. Furthermore, the hand-operated movement lever 29 can be used to move the plunger drive ram in either the forward or reverse directions; however, the range of movement speeds that can be generated with the hand-operated movement control is substantially narrowed as compared to those available in regions 1, 2a or 2b. This permits fine-tuned control of fluid injection (or withdrawal of blood, e.g., to check patency of the catheter) using the hand-operated movement control.

Regions 3a and 3b can also be used to perform injection. It may be necessary to use power head tilt angles in these regions if an obese patient or other obstacle prevents the operator from rotating the power head 22 to a fully downward position in region 4. However, since operation in regions 3a and 3b is not advisable, due to the chance that air might be injected into the subject, the operator is prevented from injecting in these regions until a software override is entered via the console touch screen 32. Until this override is

entered, the display 30 flashes and the injector  
will not perform programmed injections. Once the  
software override has been entered, the display will  
cease flashing and programmed injections can be  
5 performed. Also, as in region 4, the hand-operated  
movement lever 19 can be used to move the plunger  
drive ram in either the forward or reverse  
directions, with a narrow range of movement speeds,  
permitting fine-tuned control of fluid injection (or  
10 withdrawal) using the hand-operated movement  
control.

The various angular regions noted above,  
are also associated with display orientations.  
Specifically, as can be seen in Figs. 13B and 13C,  
15 the display 30 of the power head 22 is a segmented  
display, including segments which can be illuminated  
to provide injection information such as volume  
injected, volume remaining, and current flow rate.  
These segments are arranged so the noted information  
20 can be displayed in either a first (see Fig. 13B) or  
second (see Fig. 13C) orientation.

CPU 175 in the power head 22 drives  
display 30 to produce the display orientation, using  
the display elements in the manner illustrated in

Fig. 13C, when the power head angle is in regions 1,  
2a or 2b. Otherwise, in regions 3a, 3b or 4, CPU  
175 drives display 30 to produce the display shown  
in Fig. 13B. As a result, the information appearing  
on the display 30 is always upright from the  
perspective of the operator, facilitating use of the  
display. (There is a hysteresis included in the  
detection of the boundaries between the various  
regions shown in Fig. 13A, to prevent unintended  
toggling between regions.)

While the present invention has been  
illustrated by a description of various embodiments  
and while these embodiments have been described in  
considerable detail, it is not the intention of the  
applicant to restrict or in any way limit the scope  
of the appended claims to such detail. Additional  
advantages and modifications will readily appear to  
those skilled in the art. For example, the control  
circuit could produce an injection pressure or fill  
vacuum proportional to the extent of angular  
displacement of control lever 29 away from the home  
position, rather than a velocity proportional to the  
extent of rotation. Air bubble detection may be  
performed by an ultrasonic source and ultrasonic

69-04860

detector coupled to the neck of the syringe, in  
which case air can be detected from the large  
attenuation of sound in air as compared to fluid.  
The air bubble detector might be mounted on  
5 locations on the syringe other than on the neck.  
Also, the air bubble detector may be used in  
connection with the power head control circuitry to  
perform an automatic syringe-filling function, e.g.,  
to detect when air has been evacuated from the  
10 syringe after filling. Also, a fully pixilated  
display might be used on the power head 22, and  
controlled by the power head CPU to produce various  
orientations of display, not limited to upright and  
inverted display orientations. The invention in its  
15 broader aspects is therefore not limited to the  
specific details, representative apparatus and  
method, and illustrative example shown and  
described. Accordingly, departures may be made from  
such details without departing from the spirit or  
20 scope of applicant's general inventive concept.

What is claimed is:

Claims

1. An injector for injecting fluids from a syringe into an animal subject, having an air detector for detecting the presence of an air passing from said syringe to said animal subject, said injector comprising:

a plunger drive ram,

a motor for moving said plunger drive ram,

a syringe mounting for attachment to a syringe to position a syringe relative to said injector to permit said plunger drive ram to engage and move a plunger within said syringe,

an air detector positioned in spaced relation to said plunger drive ram to engage a wall of said syringe, said air detector including a signal source emitting an air detecting signal for transit through fluid or air contained within said syringe, a signal receiver for detecting said air detecting signal after transit through fluid or air contained within said syringe, said air detector generating a warning signal if the air detecting signal received by said signal receiver indicates the presence of air within said syringe, and

a control circuit controlling said motor to move said ram and plunger to inject fluid from said syringe, said control circuit responding to said warning signal by preventing movement of said ram to prevent air from being injected into said subject.

2. The injector of claim 1 wherein said signal source is a light emitting diode, and said air detecting signal is an electromagnetic signal.

3. The injector of claim 1 wherein said signal source is an ultrasonic transducer, and said air detecting signal is an acoustic signal.

4. The injector of claim 1 wherein said injector further comprises a housing, said syringe being mountable extending external to said housing, and said injector further comprises a post extending outwardly from said housing, said air detector being mounted to said post.

5. The injector of claim 4 further comprising a syringe having a cylindrical barrel, a plunger snugly slidable in said cylindrical barrel, a discharge tip in fluid communication with said cylindrical barrel, and a outwardly-projecting section positioned on said discharge tip,

wherein said syringe, when mounted to said injector, presses said outwardly-projecting section against said air detector, to facilitate transmission of said air detecting signal into said discharge tip of said syringe.

6. The injector of claim 5 wherein said outwardly-projecting section of said syringe is a circumferential collar surrounding said discharge tip.

7. The injector of claim 5 wherein said signal source is a light emitting diode, and said air detecting signal is an electromagnetic signal, said syringe being configured to substantially reflect said electromagnetic signal from an interior wall of said discharge tip and toward said signal

receiver only when said discharge tip contains fluid.

8. A syringe for mounting to an injector having an air detector, said syringe comprising:

a cylindrical barrel,

a plunger snugly slidable in said cylindrical barrel,

a discharge tip in fluid communication with said cylindrical barrel, and

a outwardly-projecting section positioned on said discharge tip, said section being configured to substantially transmit an air detecting signal received externally of said section into an interior of said discharge tip for reflection from an interior wall of said discharge tip back through said section.

9. The syringe of claim 8 wherein said outwardly-projecting section of said syringe is a circumferential collar surrounding said discharge tip.

10. The syringe of claim 9 wherein said collar has a concave cross section and forms a lens for focussing light received from external to said collar into said discharge tip of said syringe.

11. An injector for injecting fluids from a syringe into an animal subject, having a hand-operated movement control for controlling movements of said injector, said injector comprising:

a plunger drive ram,

a motor for moving said plunger drive ram,

a syringe mounting for attachment to a syringe to position a syringe relative to said injector to permit said plunger drive ram to engage and move a plunger into or out of said syringe,

a control circuit controlling said motor to move said ram and plunger to inject fluid from said syringe, and

a hand-operated movement control comprising a lever movable between a home position and forward and reverse positions,

said control circuit responding to movement of said lever to a forward position by

moving said plunger drive ram into said syringe to expel fluid from the syringe, said control circuit responding to movement of said lever to a reverse position by moving said plunger drive ram out of said syringe to draw fluid into the syringe.

12. The injector of claim 11 wherein said lever is mounted in said injector on a pivot shaft, and further comprising return springs positioned on opposite sides of said lever such that rotation of said lever away from said home position bends said return springs.

13. The injector of claim 12 further comprising a rotational detector attached to said pivot shaft for rotation with said lever to detect an angle of rotation of said lever to produce a rotation angle signal, wherein said control circuit responds to said rotation angle signal by moving said plunger drive ram at a speed related to said rotation angle signal.

14. The injector of claim 13 wherein said control signal moves said plunger drive ram at a speed proportionate to said angle of rotation of said lever.

15. The injector of claim 13 wherein said rotational detector is a rotary potentiometer.

16. The injector of claim 12 further comprising a rotational detector attached to said pivot shaft for rotation with said lever to detect an angle of rotation of said lever to produce a rotation angle signal, wherein said control circuit responds to said rotation angle signal by moving said plunger drive ram so as to generate an injection pressure related to said rotation angle signal.

17. The injector of claim 12 wherein said return springs and said lever are electrical contacts, and further comprising a safety circuit generating a safety control signal indicating

whether there is electrical contact between said  
return springs and said lever,

said control circuit responding to said  
safety control signal,

whereby the failure of a return spring is  
electrically detectable by said control circuit.

18. The injector of claim 12 further  
comprising a detent spring positioned relative to  
said lever to engage said lever upon rotation of  
said lever into a position which is more than a  
predetermined angle from said home position, said  
detent spring producing additional resistive torque  
opposing rotation of said lever away from said home  
position beyond said predetermined angle.

19. The injector of claim 18 wherein said  
detent spring is positioned relative to said lever  
to engage said lever upon rotation of said lever to  
a reverse position.

20. The injector of claim 19 wherein said  
detent spring and said lever are electrical

contacts, further comprising a detent circuit generating a detent signal indicating whether there is electrical contact between said detent spring and said lever,

said control circuit responding to said detent signal by moving said plunger drive ram out of said syringe to draw fluid into said syringe at said predetermined recommended maximum speed.

21. An injector for injecting fluids from a syringe into an animal subject, comprising:

a plunger drive ram,

a motor for moving said plunger drive ram,

a syringe mounting for attachment to a syringe to position a syringe relative to said injector to permit said plunger drive ram to engage and move a plunger into or out of said syringe,

an electronic display displaying information regarding the activities and state of operation of said injector, said display capable of displaying information in at least a first and a second orientation,

a tilt sensor generating a tilt angle signal indicative of an angle of tilt of said injector relative to the direction of Earth gravitation, and

a control circuit connected to said motor and said display, controlling said motor to move said ram and plunger to inject fluid from said syringe, and generating display information and delivering said display information to said display,

wherein said display is responsive to said tilt angle signal to display said display information in said first orientation in response to a first range of values of said tilt angle signal, and to display said display information in said second orientation in response to a second range of values of said tilt angle signal.

22. The injector of claim 21 wherein said display comprises display elements arranged in positions to produce numerals in either an upright or inverted orientation.

23. The injector of claim 22 wherein said display is a light emitting diode display.

24. The injector of claim 21 wherein said display is a matrix of evenly-spaced pixels which can be selectively activated to, in combination, for graphics or characters for display.

25. The injector of claim 21 wherein said control circuit is responsive to said tilt angle signal to determine a speed of motion of said motor.

26. The injector of claim 25 wherein said control circuit operates said motor at a first speed if said tilt angle signal indicates that said injector is tilted upward with an outlet of said syringe elevated above said syringe, and said control circuit operates said motor at a second speed slower than said first speed if said tilt angle signal indicates that said injector is tilted downward with an outlet of said syringe positioned below said syringe.

27. The injector of claim 21 further comprising a hand-operated movement control connected to said control circuit for generating a movement signal, said control circuit responsive to said movement signal to cause motion of said motor in a direction indicated by said movement signal, said control circuit further responsive to stored programming to automatically move said motor to perform an injection,

wherein said control circuit is responsive to said tilt angle signal to inhibit automatic movement of said motor in response to stored programming unless said tilt angle signal indicates that said injector is tilted within a predetermined range of angles relative to Earth gravitation.

28. The injector of claim 21 wherein said control circuit is further responsive to said tilt angle signal to generate display information warning an operator against performing an injection if said tilt angle signal indicates that said injector is tilted within a predetermined range of angles relative to Earth gravitation.

29. An injector for injecting fluids from a syringe into an animal subject, comprising:

a plunger drive ram,

a motor for moving said plunger drive ram,

a syringe mounting for attachment to a syringe to position a syringe relative to said injector to permit said plunger drive ram to engage and move a plunger into or out of said syringe,

a tilt sensor generating a tilt angle signal indicative of an angle of tilt of said injector relative to the direction of Earth gravitation, and

a control circuit connected to said motor and controlling said motor to move said ram and plunger to inject fluid from said syringe, said control circuit being responsive to said tilt angle signal to determine a speed of motion of said motor.

30. The injector of claim 29 wherein said control circuit operates said motor at a first speed if said tilt angle signal indicates that said injector is tilted upward with an outlet of said syringe elevated above said syringe, and said

control circuit operates said motor at a second speed which is slower than said first speed if said tilt angle signal indicates that said injector is tilted downward with an outlet of said syringe positioned below said syringe.

31. The injector of claim 29 further comprising a hand-operated movement control connected to said control circuit for generating a movement signal, said control circuit responsive to said movement signal to cause motion of said motor in a direction indicated by said movement signal, said control circuit further responsive to stored programming to automatically move said motor to perform an injection,

wherein said control circuit is responsive to said tilt angle signal to inhibit automatic movement of said motor in response to stored programming unless said tilt angle signal indicates that said injector is tilted within a predetermined range of angles relative to Earth gravitation.

32. The injector of claim 29 wherein said control circuit is further responsive to said tilt angle signal to generate display information warning an operator against performing an injection if said tilt angle signal indicates that said injector is tilted within a predetermined range of angles relative to Earth gravitation.

33. An injector for injecting fluids from a syringe into an animal subject, comprising:

a housing,

a plunger drive ram mounted within said housing,

a motor for moving said plunger drive ram into and out of said housing,

a face plate mounting on an external surface of said housing for receiving a detachable face plate used to position a syringe relative to said injector housing to permit said plunger drive ram to engage and move a plunger into or out of said syringe, said face plate including one or more sources of magnetic field energy, the presence or absence or orientation of said sources in a given

face plate being indicative of attributes of said face plate and of a syringe type which can be mounted to said injector using said face plate,

one or more magnetic conductors of magnetically permeable material extending from said face plate mounting through said housing, positioned to channel magnetic field energy from said one or more sources into said housing, and

a control circuit connected to said motor and controlling said motor to move said ram and plunger to inject fluid from said syringe, said control circuit including one or more magnetic field detectors positioned inside said housing adjacent said magnetic conductors to detect magnetic fields channeled into said housing by said magnetic conductors, said control circuit being responsive to said magnetic field detectors to identify a face plate mounted to said injector based on the presence or absence or orientation of magnetic field energy detected by said magnetic field detectors, and to move said motor in a manner appropriate for a syringe type which can be mounted to said injector using said face plate.

04440-11099

34. An injector for injecting fluids from a syringe into an animal subject, comprising:

a plunger drive ram,

a motor for moving said plunger drive ram,

a syringe mounting for attachment to a syringe to position a syringe relative to said injector to permit said plunger drive ram to engage and move a plunger into or out of said syringe,

a hand-operated movement control for generating a movement request signal indicating movements of said plunger drive ram desired by an operator,

an encoder connected to said motor for generating a motion signal indicative of motion of said plunger drive ram,

a motor control circuit connected to said motor, said hand-operated movement control and said encoder controlling said motor to move said ram and plunger to inject fluid from said syringe, said motor control circuit being responsive to said movement request signal to instruct said motor to move said plunger drive ram, said motor control circuit further generating a state signal indicating

a state of operation of said motor control circuit for delivery through a monitor interface of said motor control circuit, said state signal indicating at least whether said motor control circuit is responding to said movement request signal by moving said motor,

a motor monitor circuit connected to said hand-operated movement control, said encoder, and said monitor interface of said motor control circuit, monitoring said movement request signal, said motion signal and said state signal, said motor monitor circuit confirming that said state signal is consistent with said movement request signal and said motion signal, by at least confirming that when said movement request signal indicates that movements of said motor are desired, and said state signal indicates said motor control circuit is responding to said movement request signal to move said motor, said motion signal indicates said motor is moving in accordance with said movement request signal.

35. The injector of claim 34 wherein said motor monitor circuit generates an alarm signal if said state signal is not consistent with said movement request signal and said motion signal.

36. The injector of claim 35 wherein said motor is responsive to said alarm signal to disable further motion of said plunger drive ram when said monitor circuit is generating said alarm signal.

37. The injector of claim 34 further comprising

a console for permitting an operator to specify a program of desired motion of said plunger drive ram,

a console control circuit connected to said console for obtaining and storing a program of desired motion specified by an operator,

said console control circuit generating said movement request signal in response to said stored program of desired motion.

38. The injector of claim 37 wherein said console control circuit generates a console state signal indicative of operation of said console control circuit, and further comprising a console monitor circuit for communicating with said console control circuit to obtain said console state signal, said console monitor circuit further communicating with said motor monitor circuit whenever said console control circuit is generating said movement request signal to confirm said motor control circuit is responding to said movement request signal as determined by said motor monitor circuit.

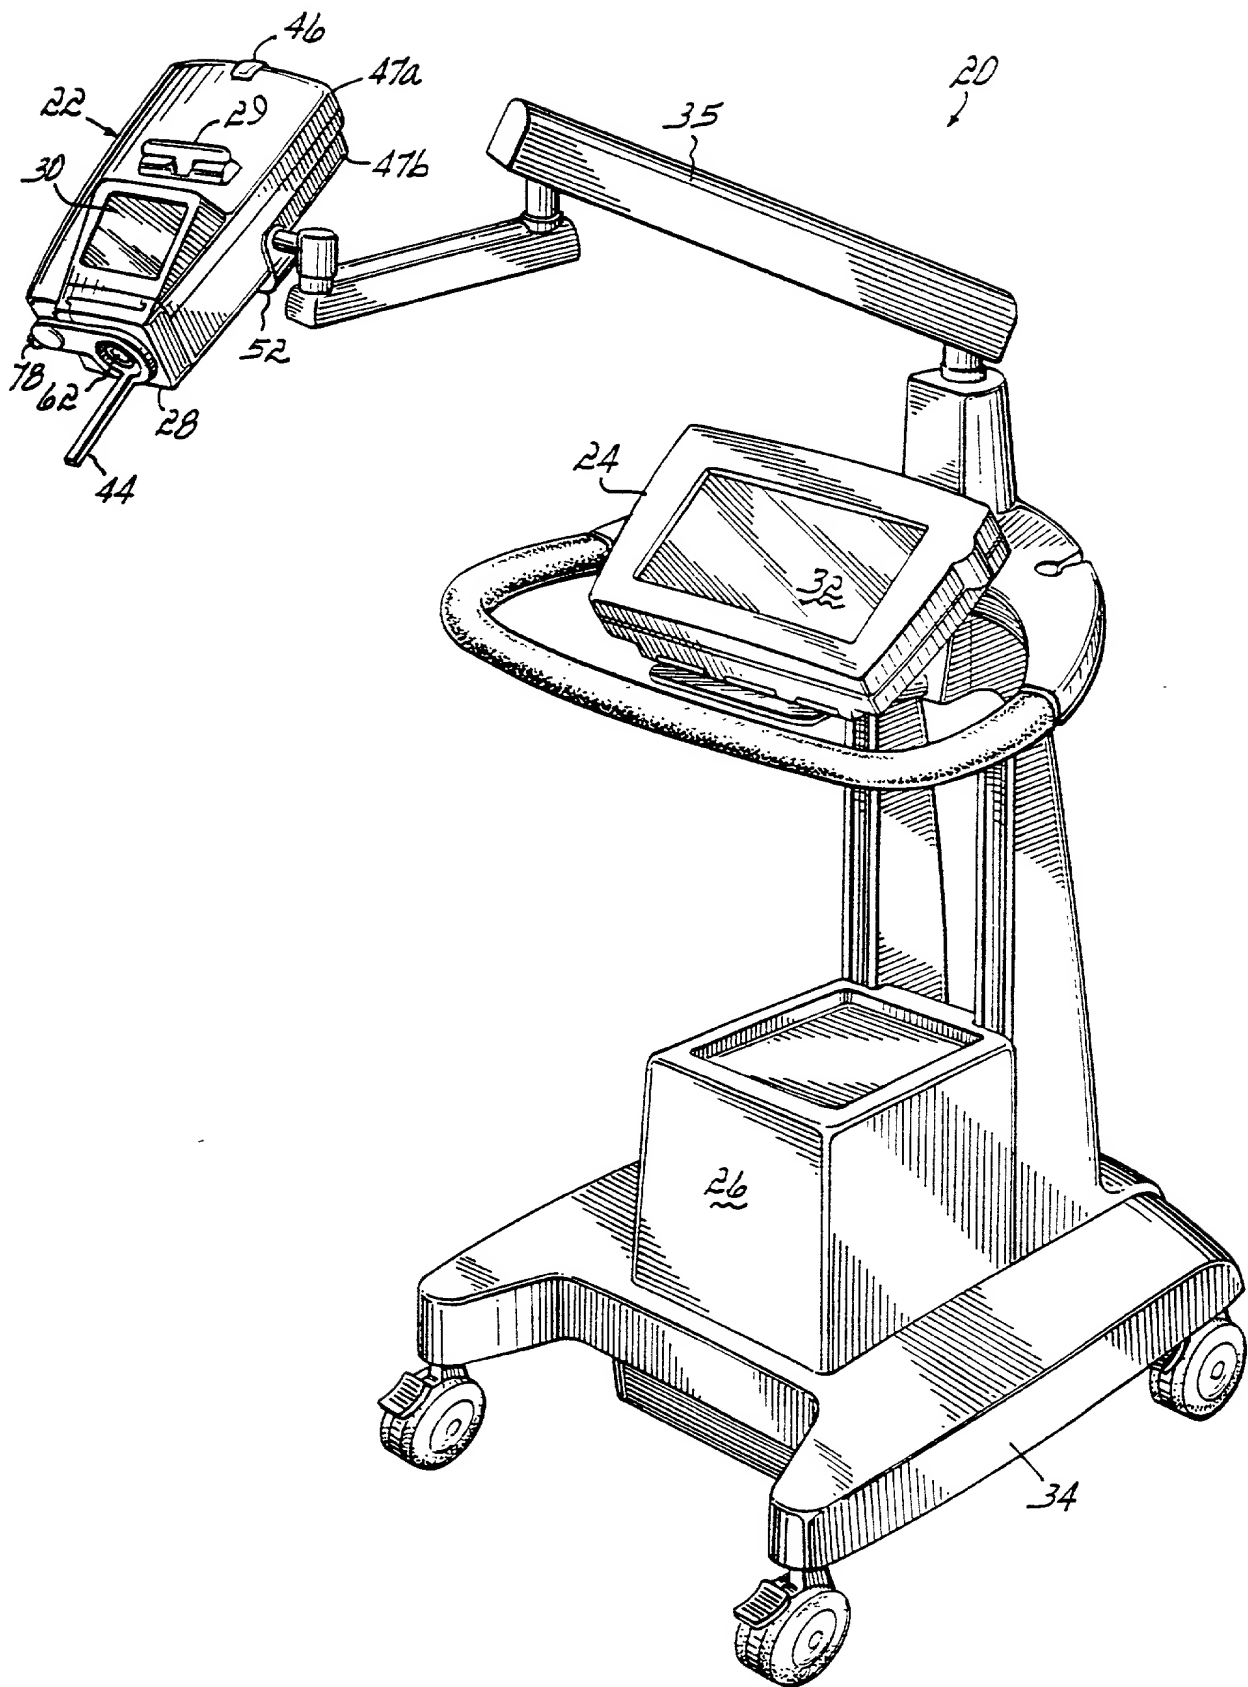
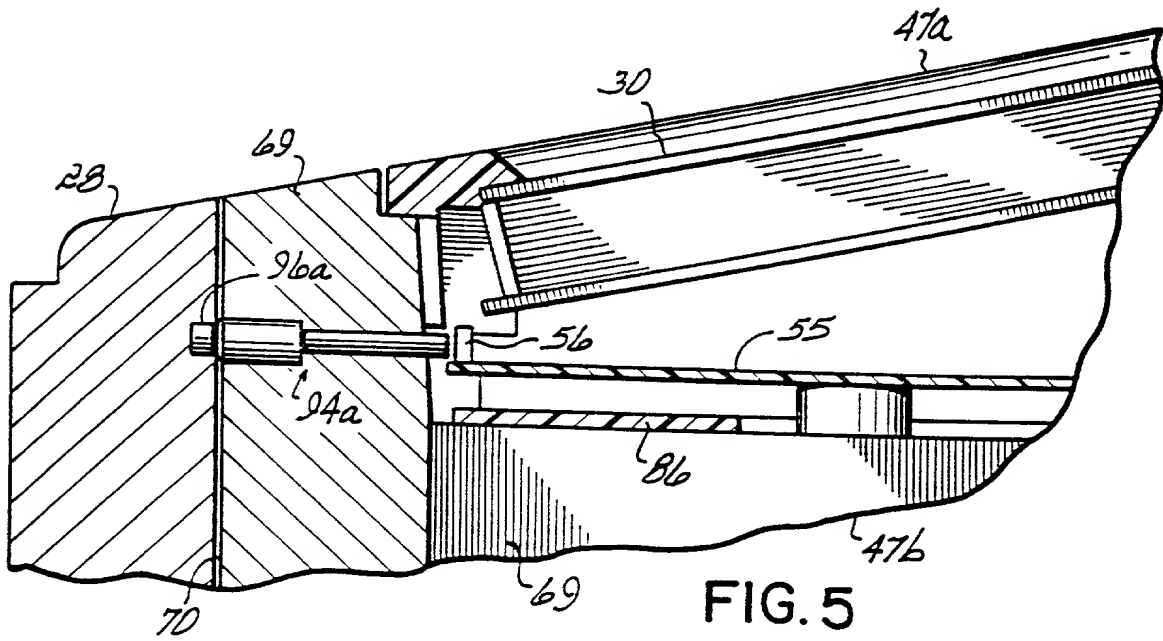
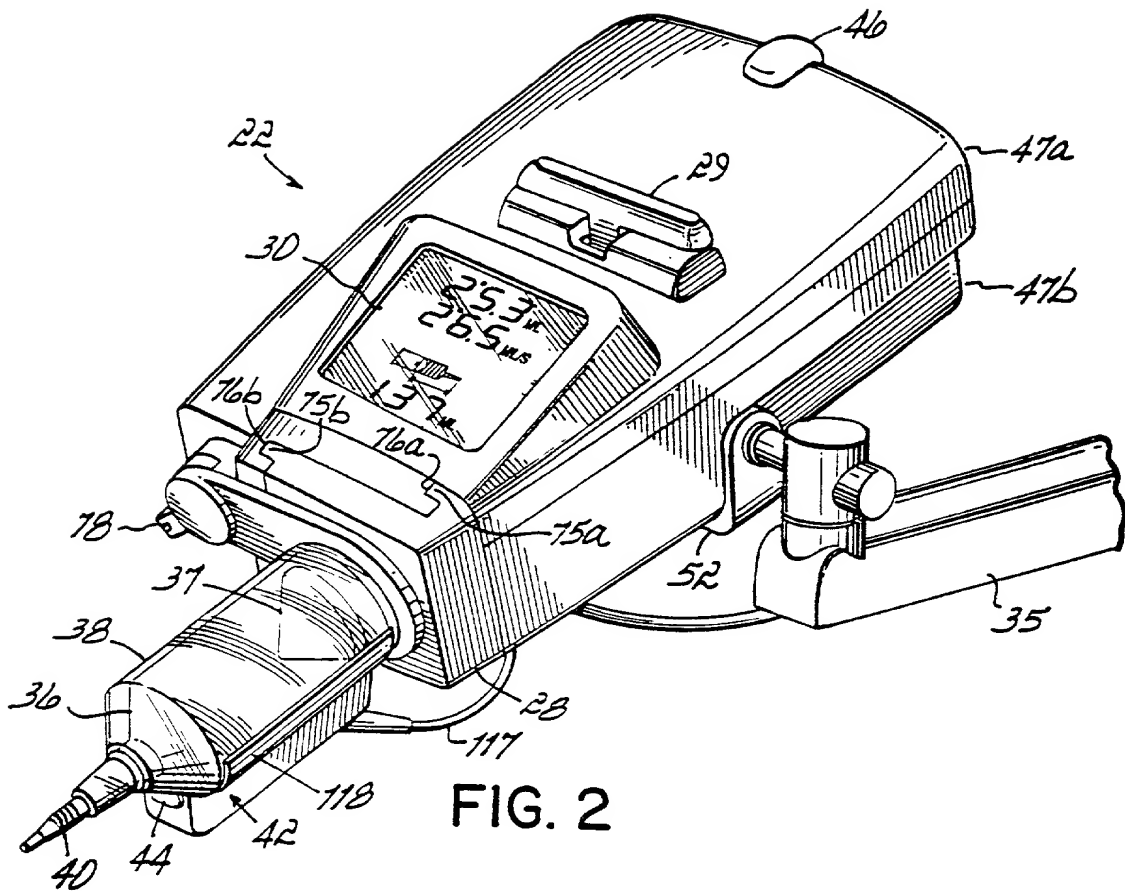


FIG. 1



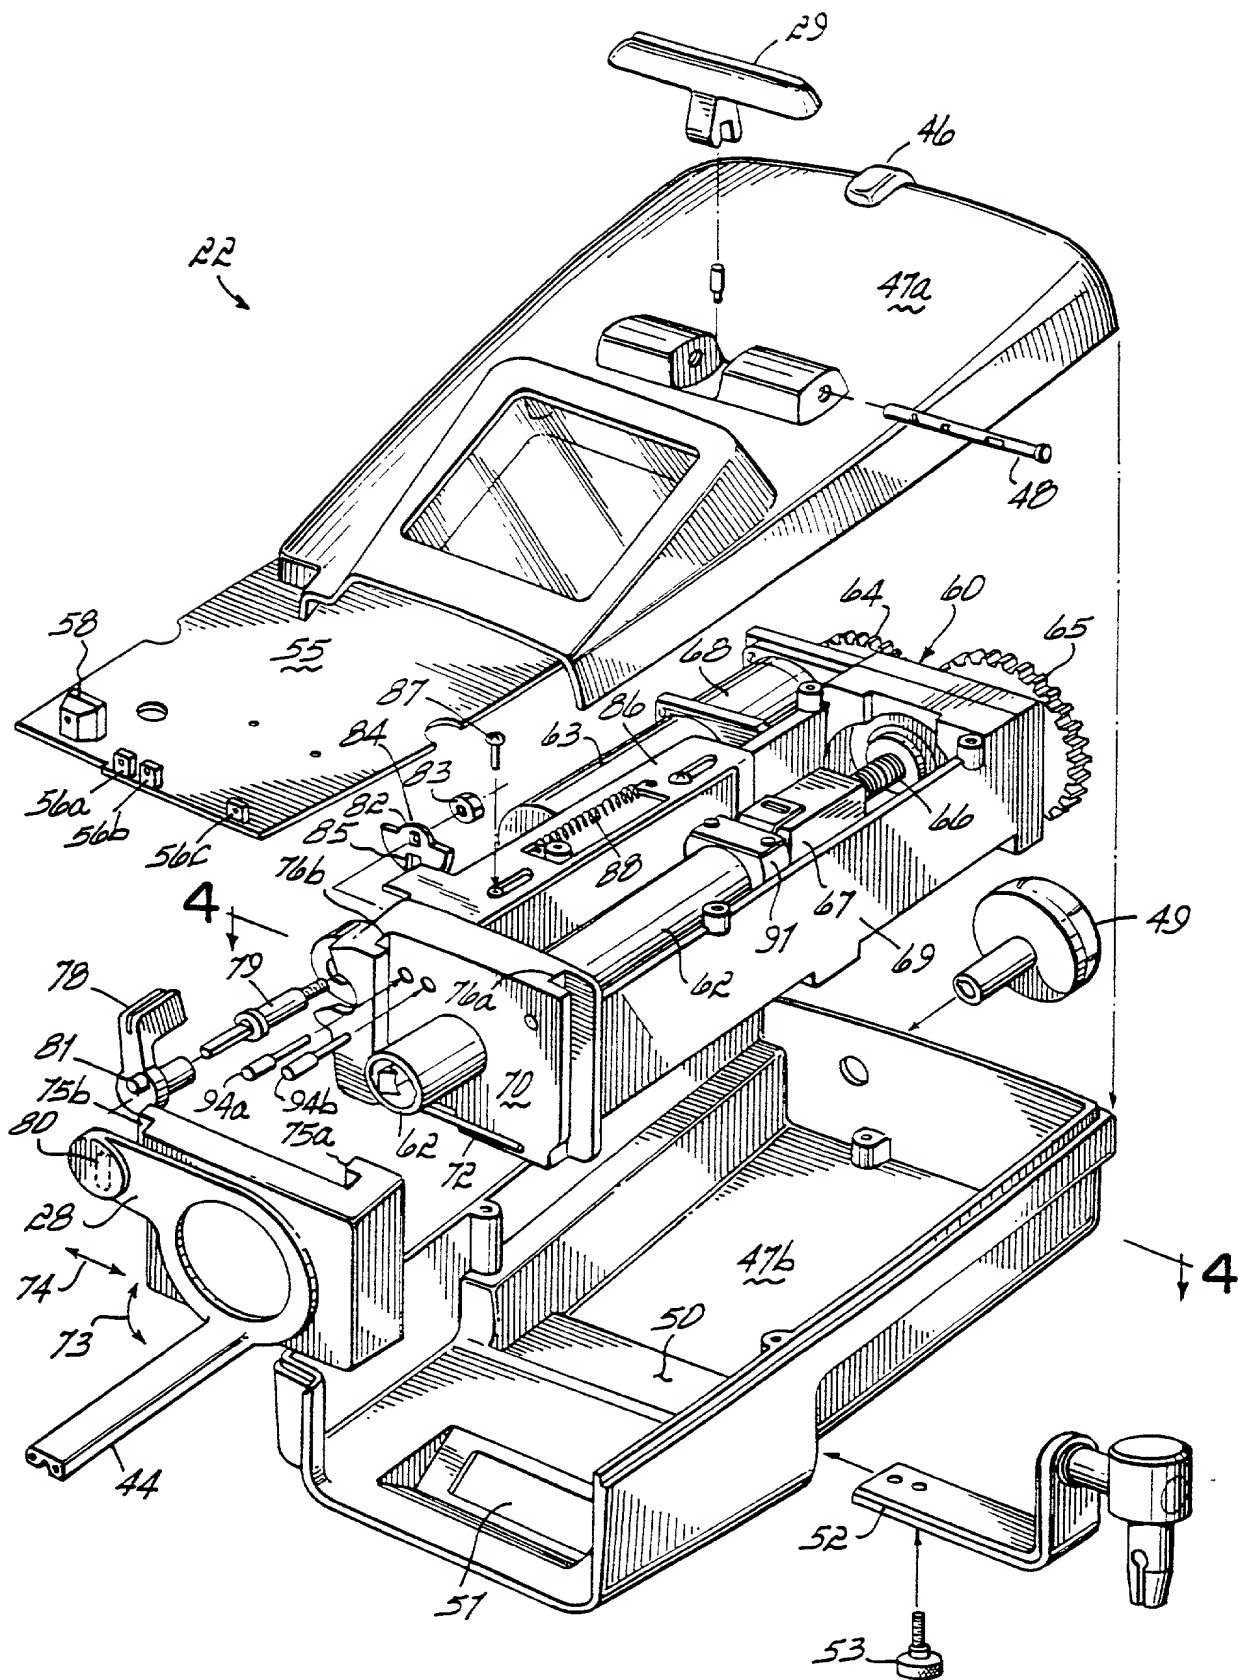
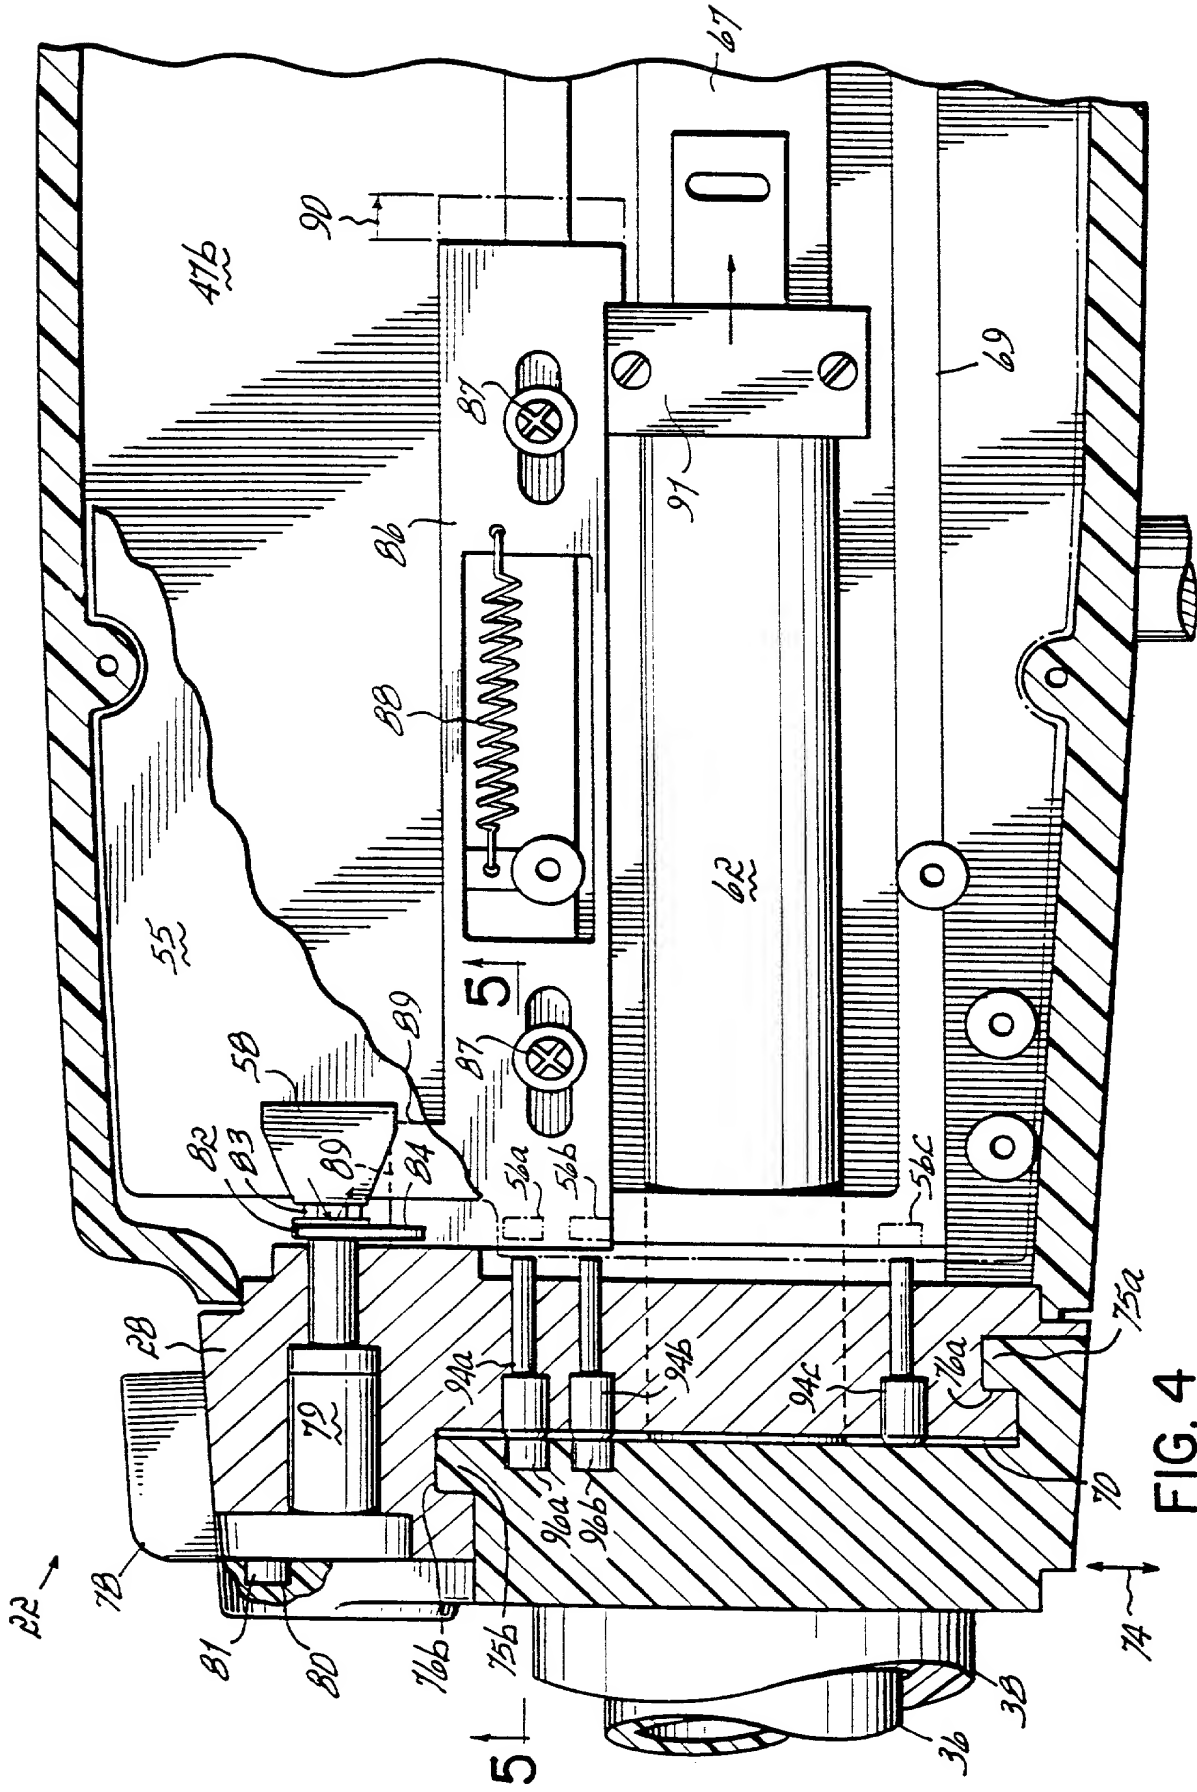


FIG. 3



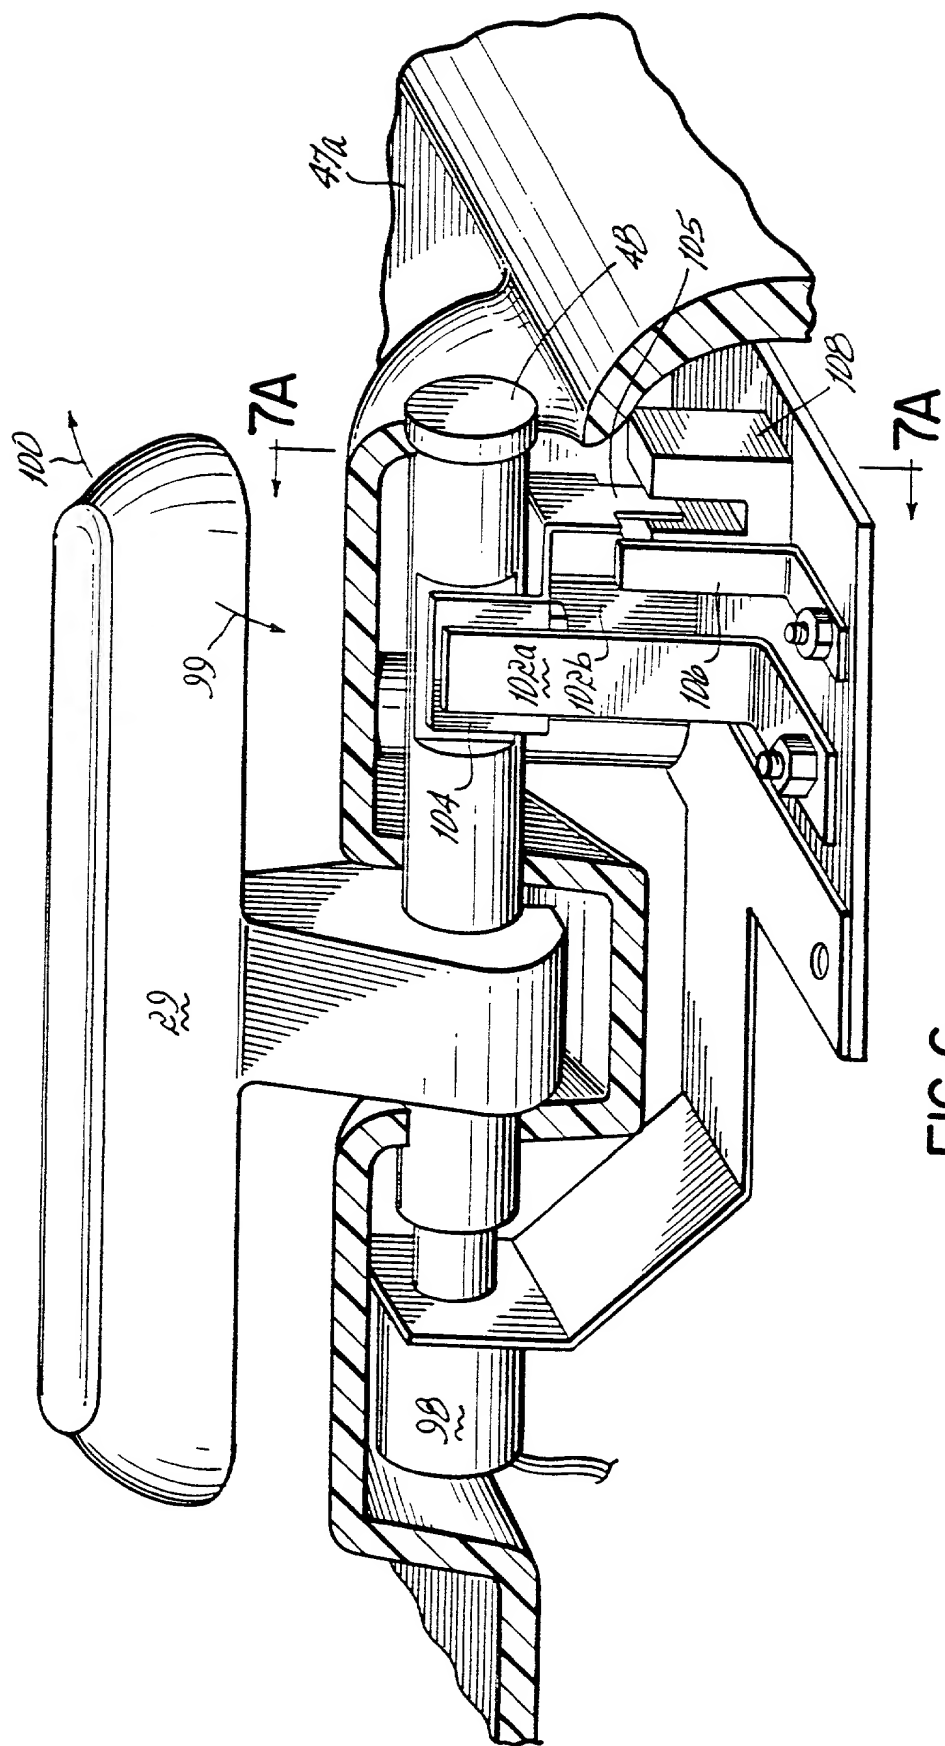
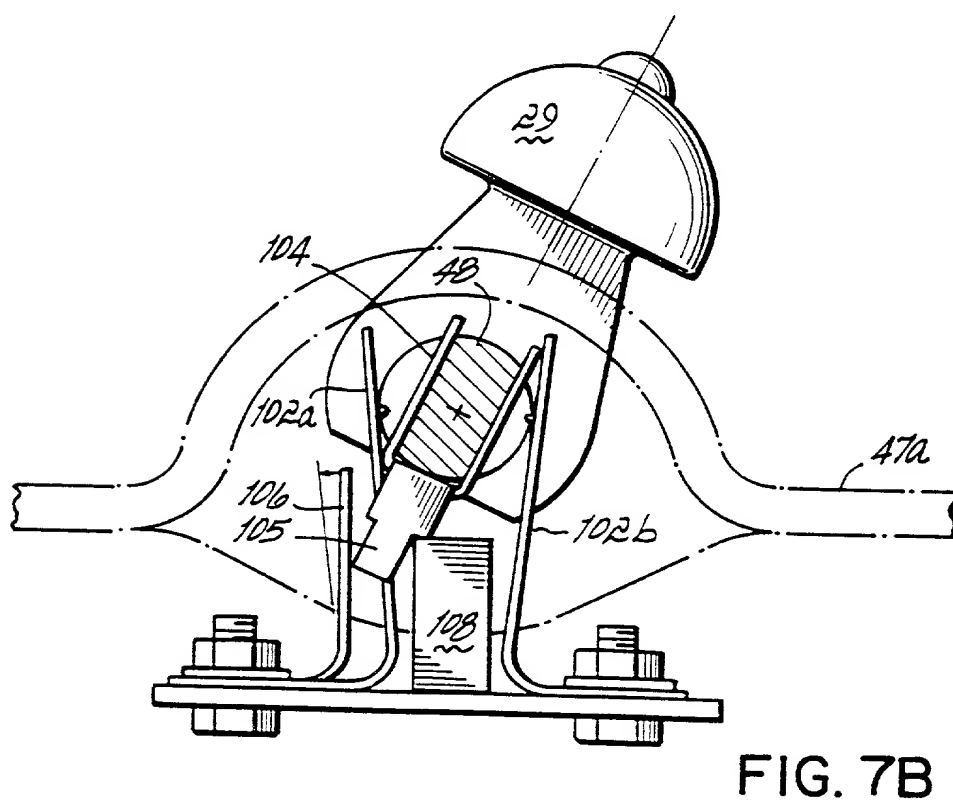
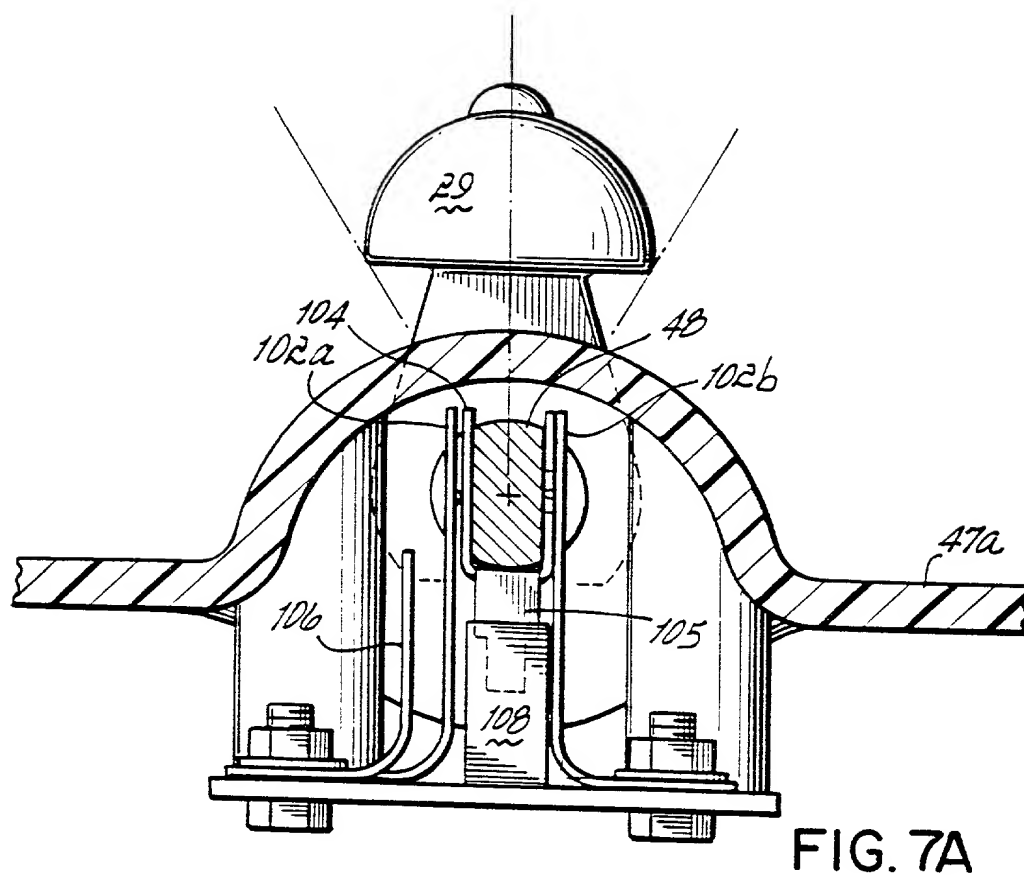


FIG. 6



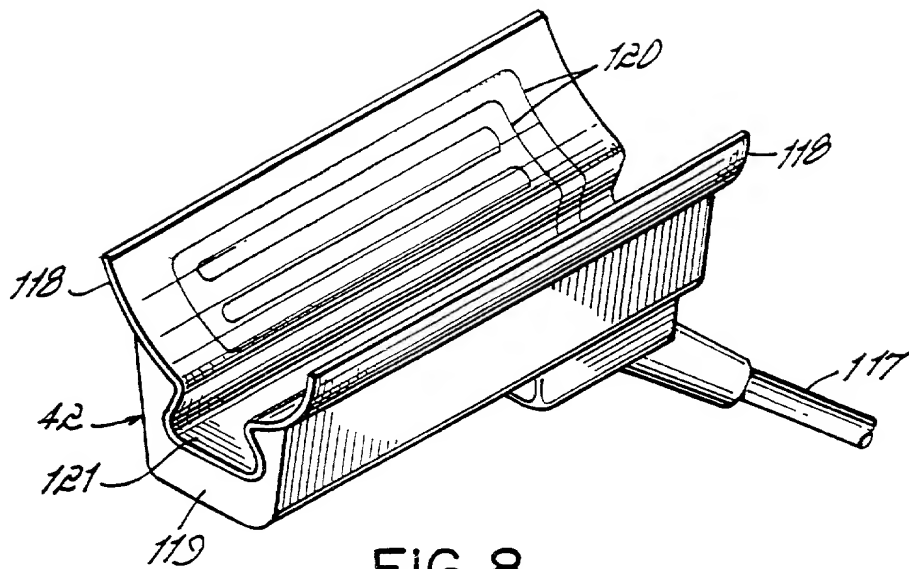


FIG. 8

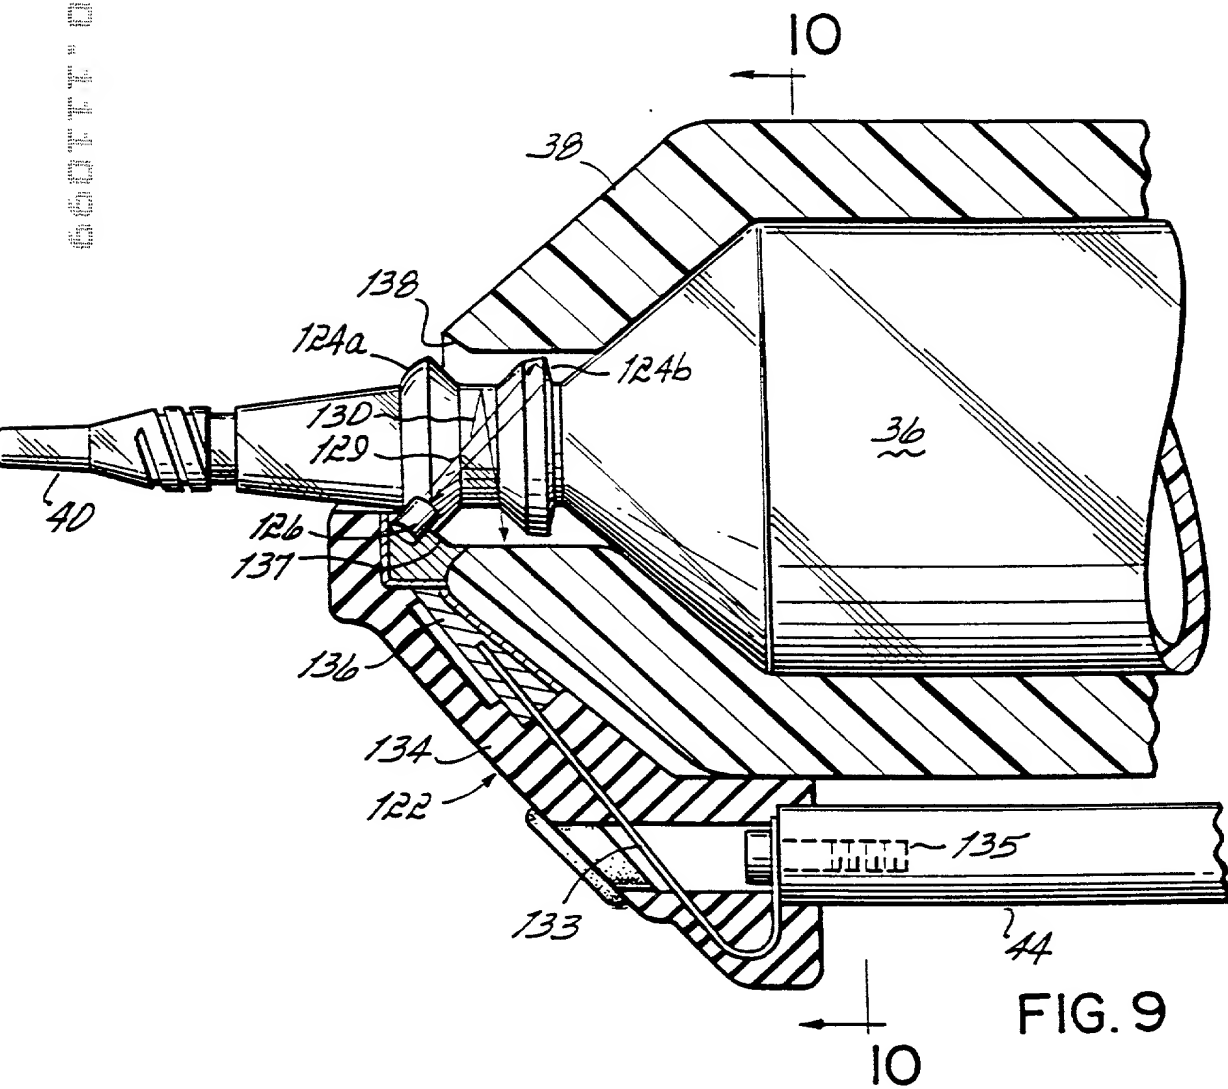


FIG. 9

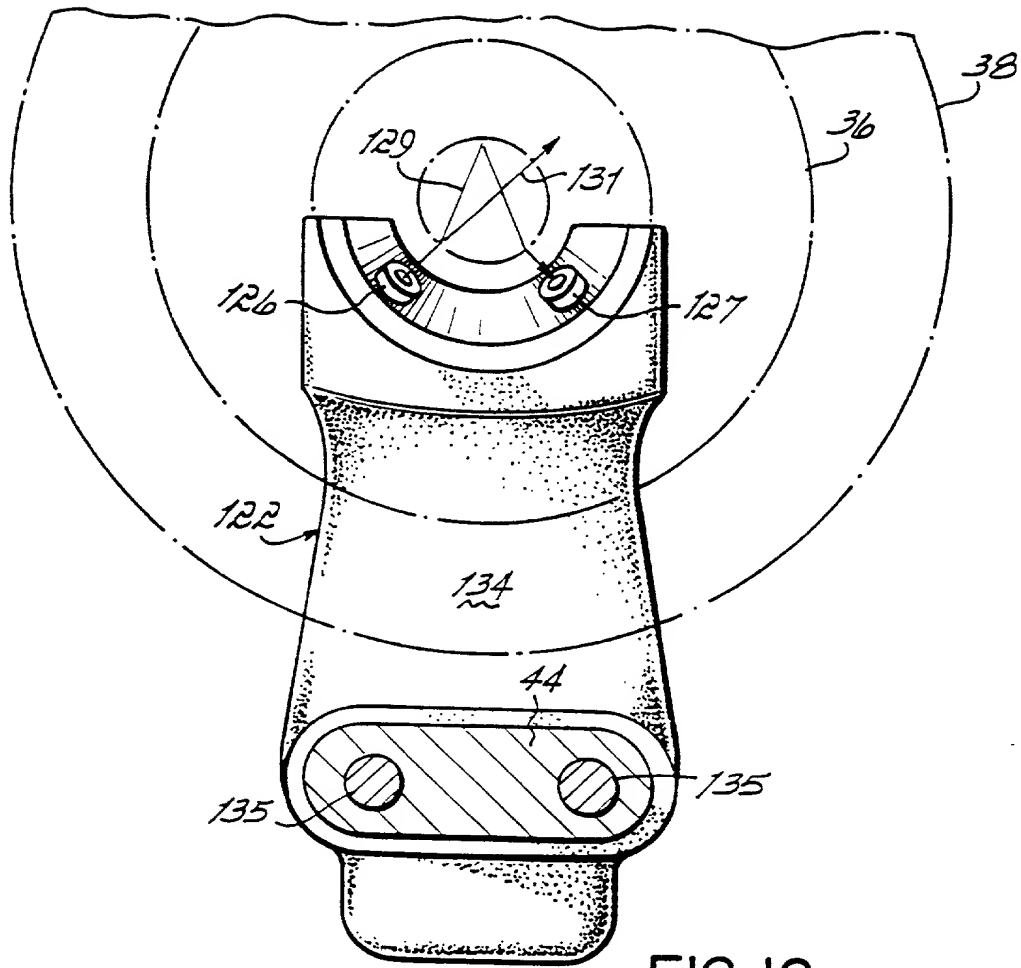
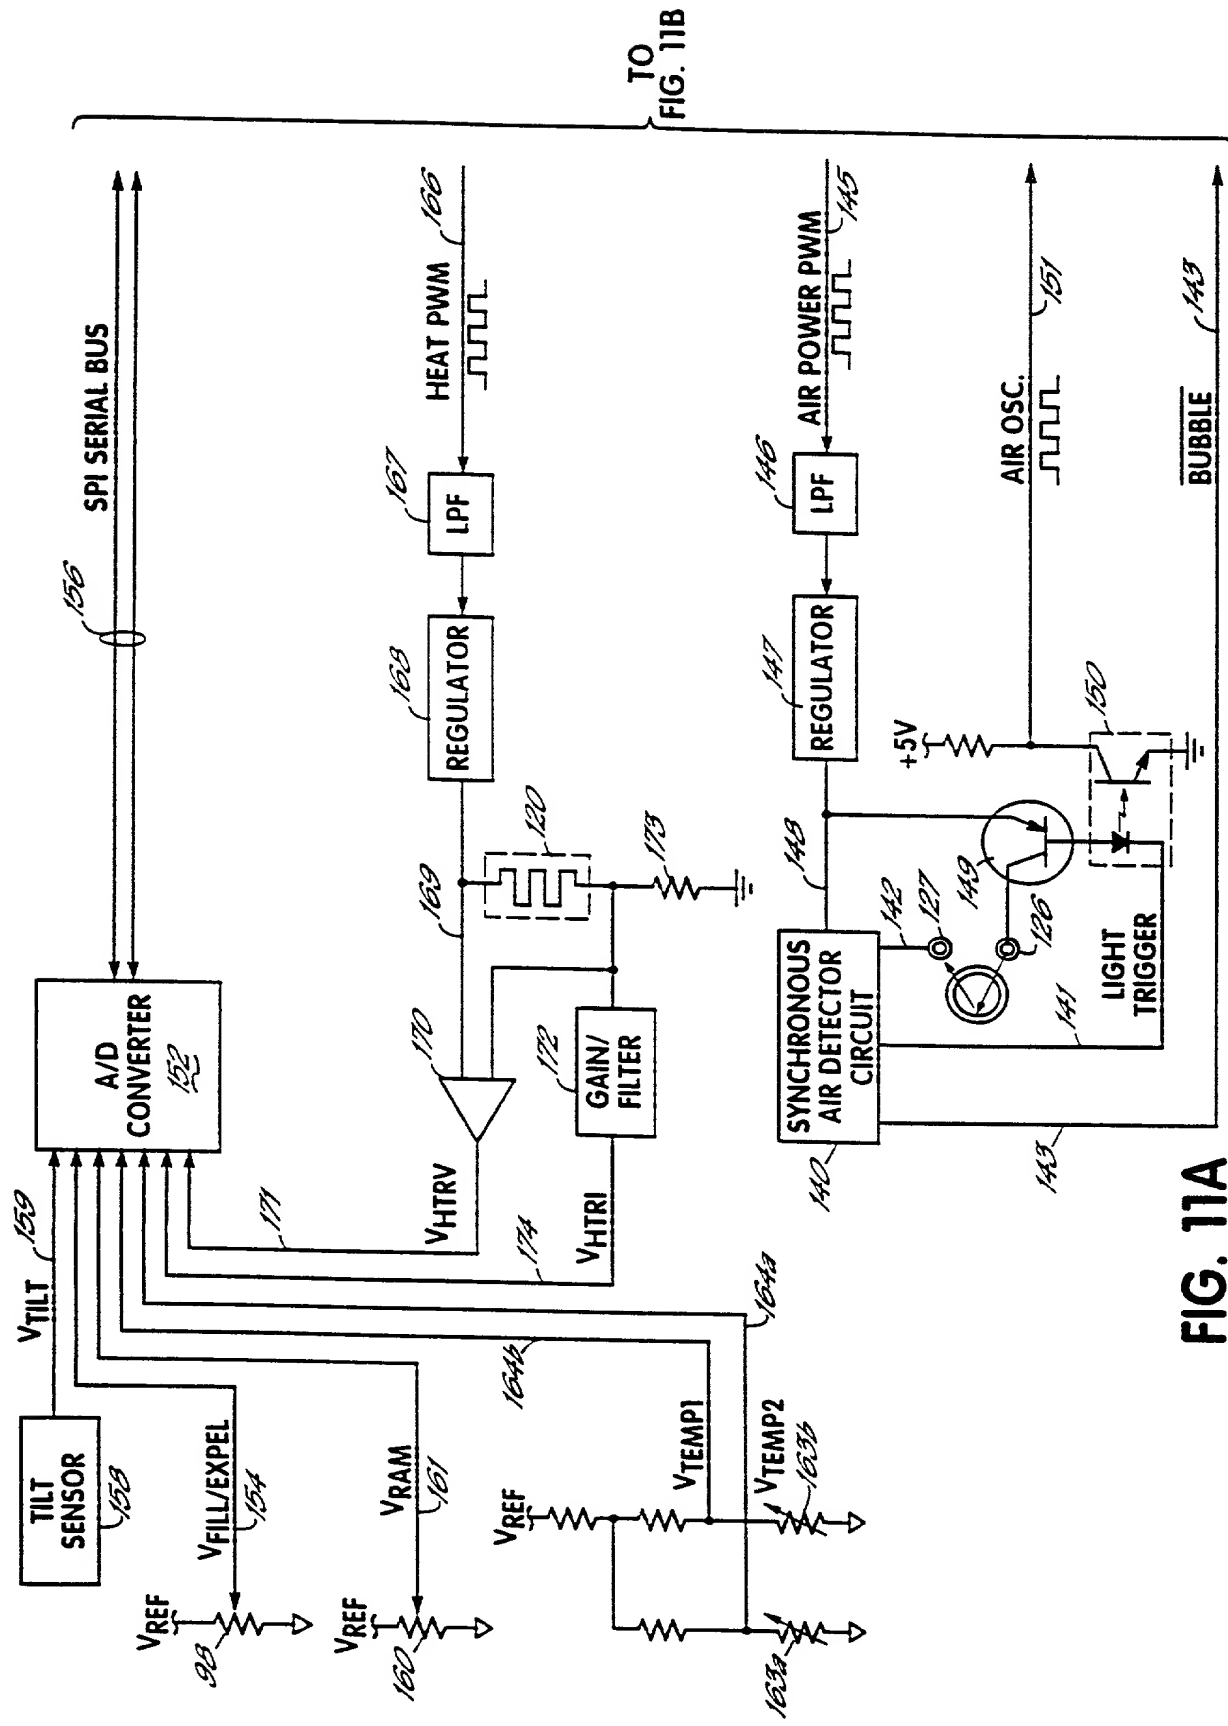


FIG. 10



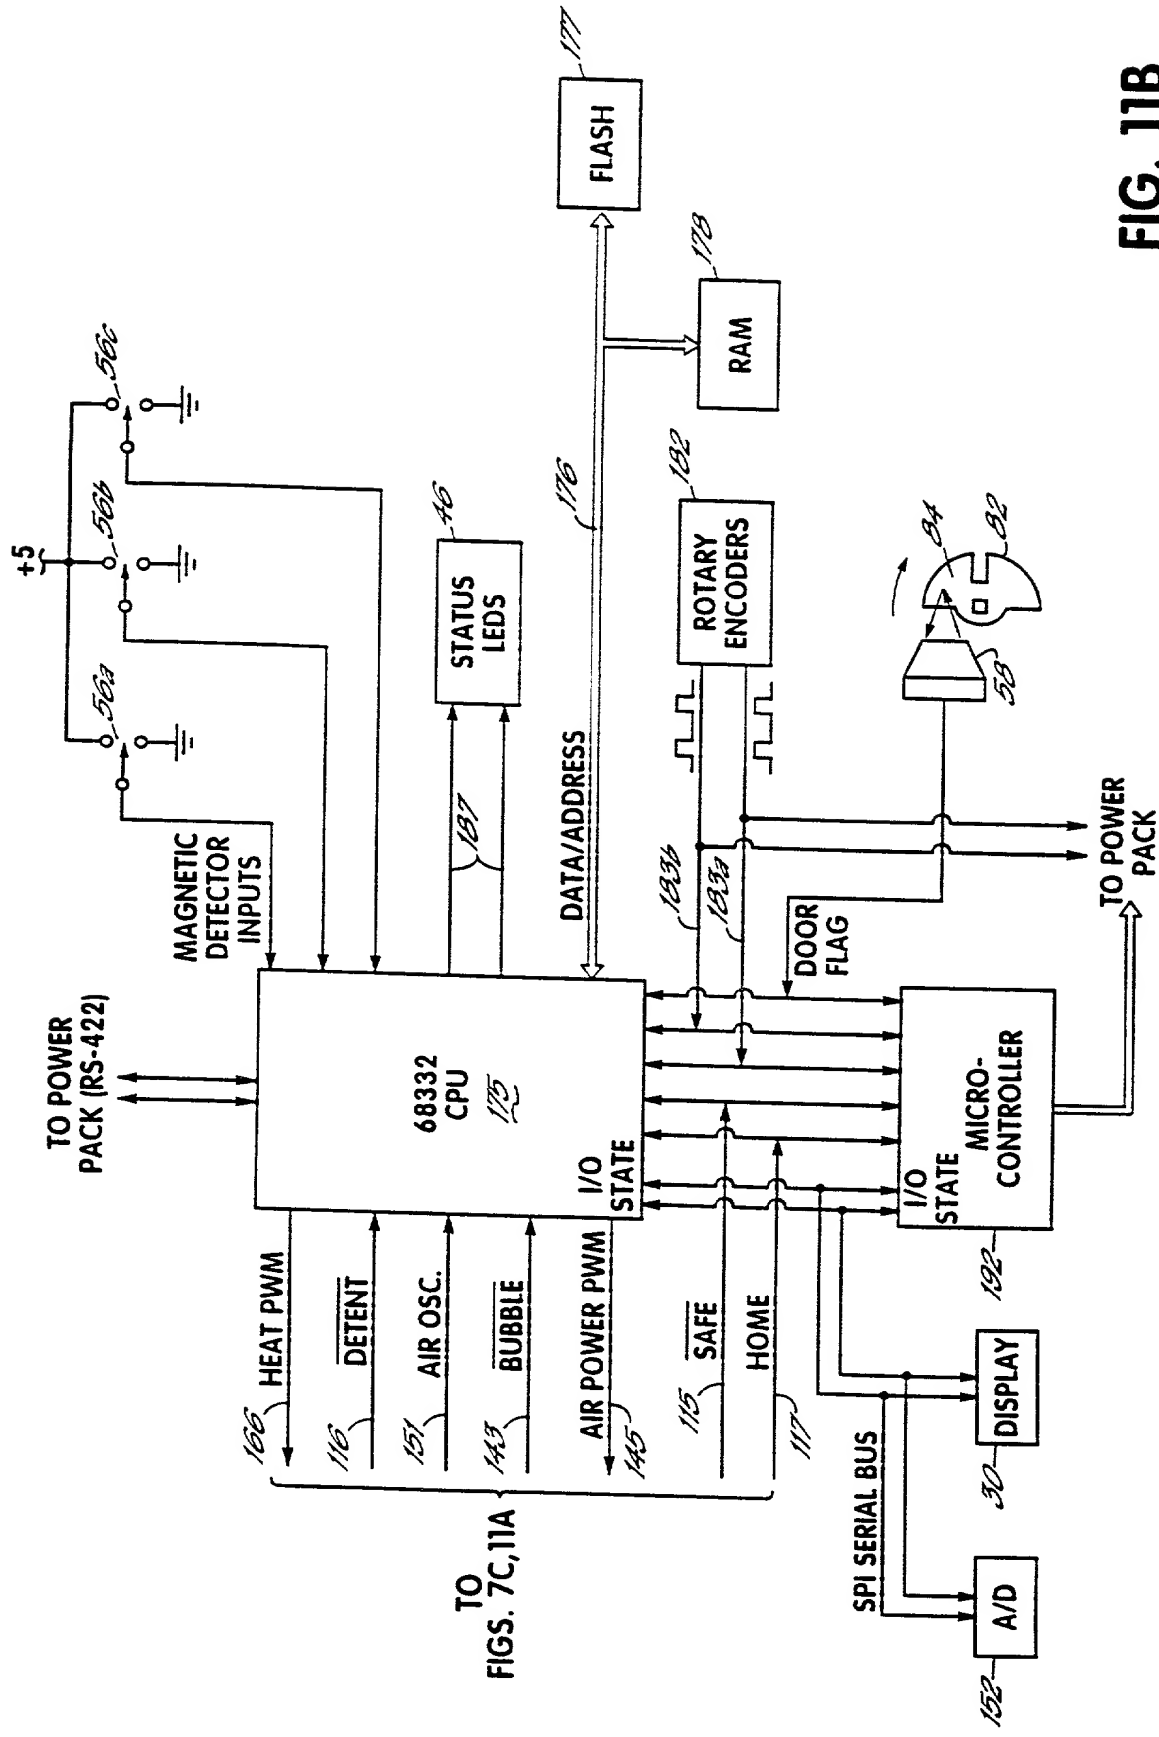


FIG. 11B

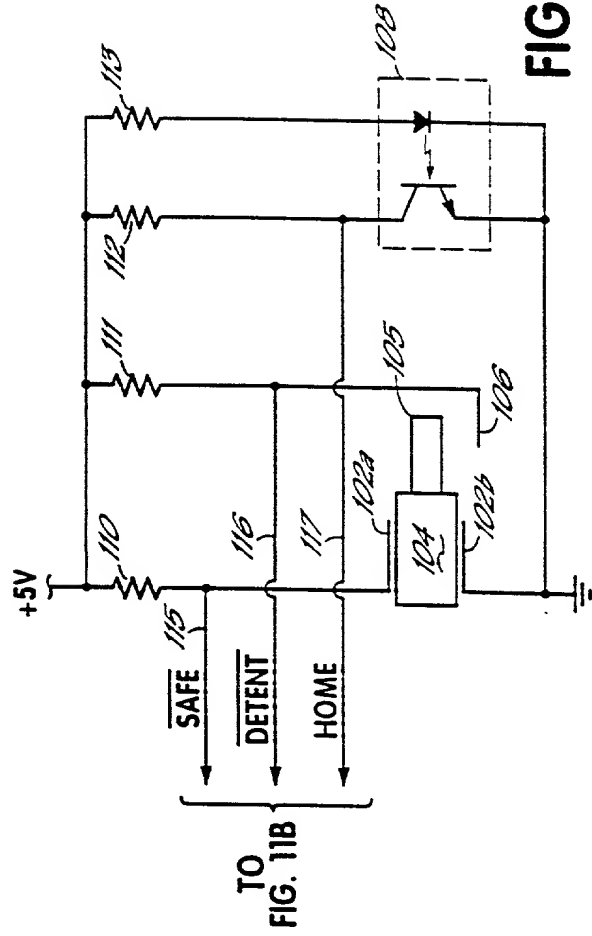


FIG. 7C

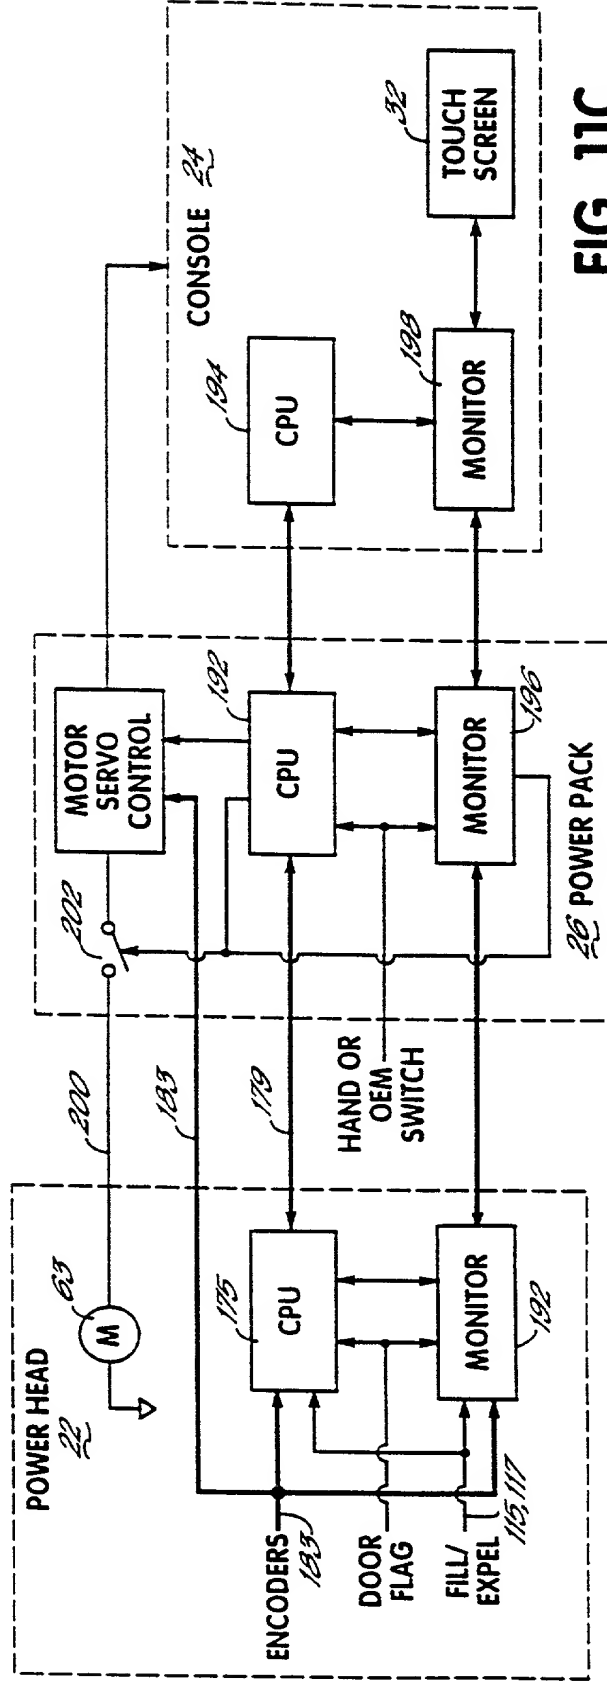


FIG. 11C

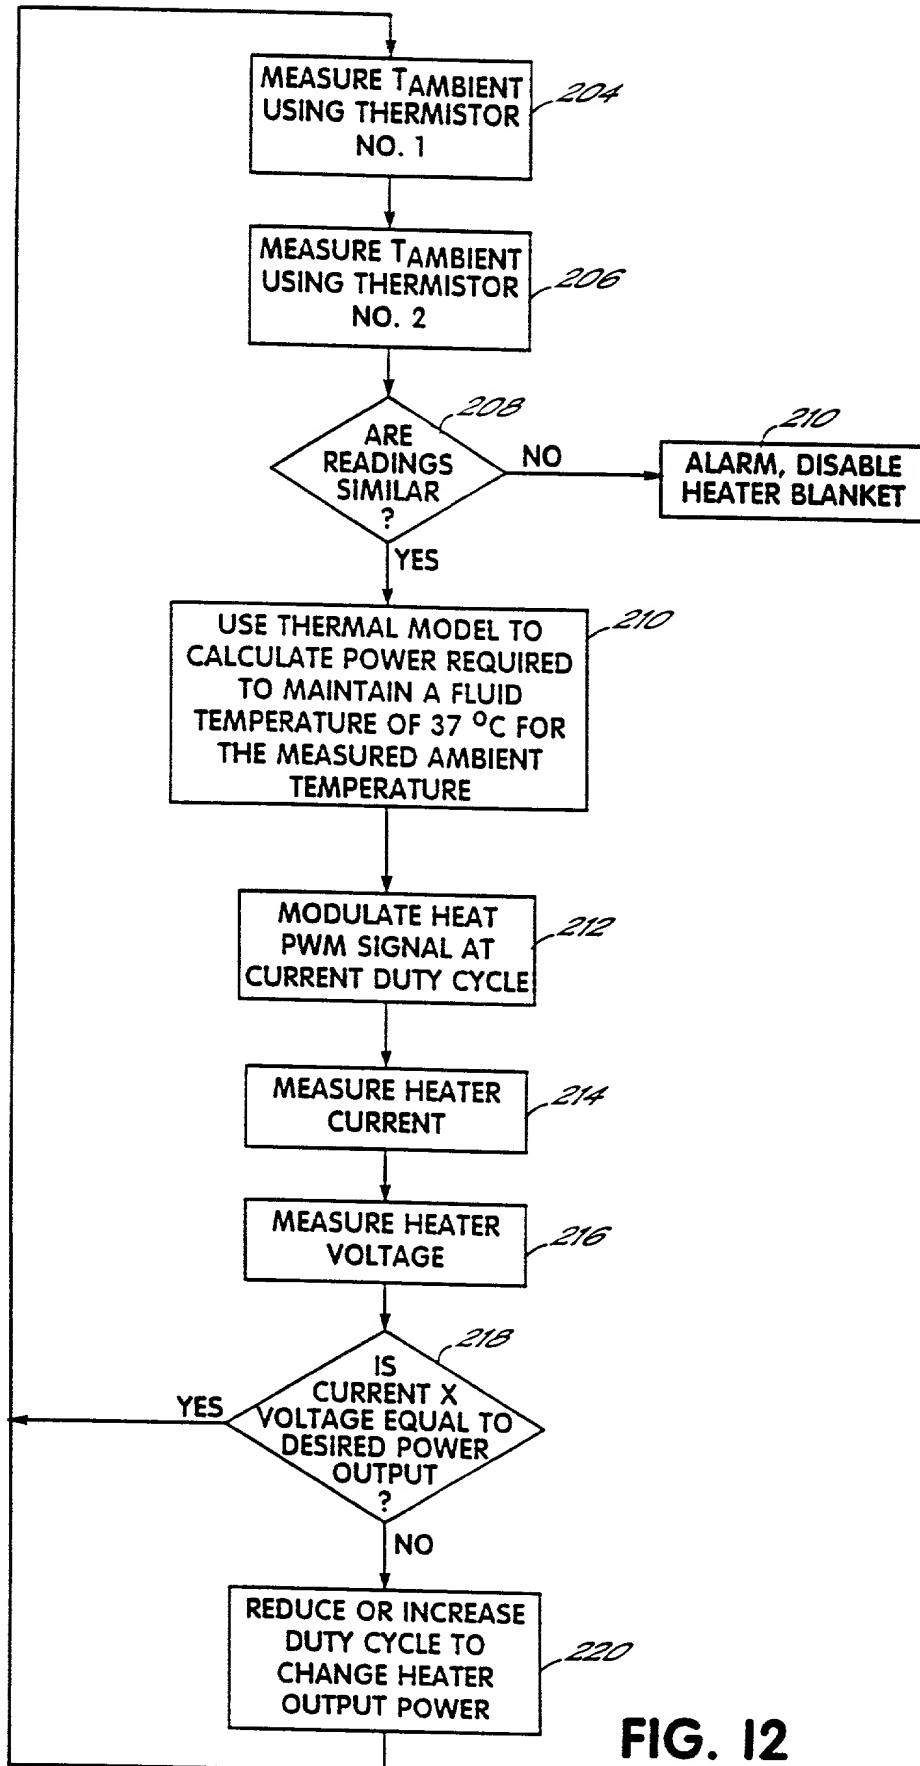


FIG. 12

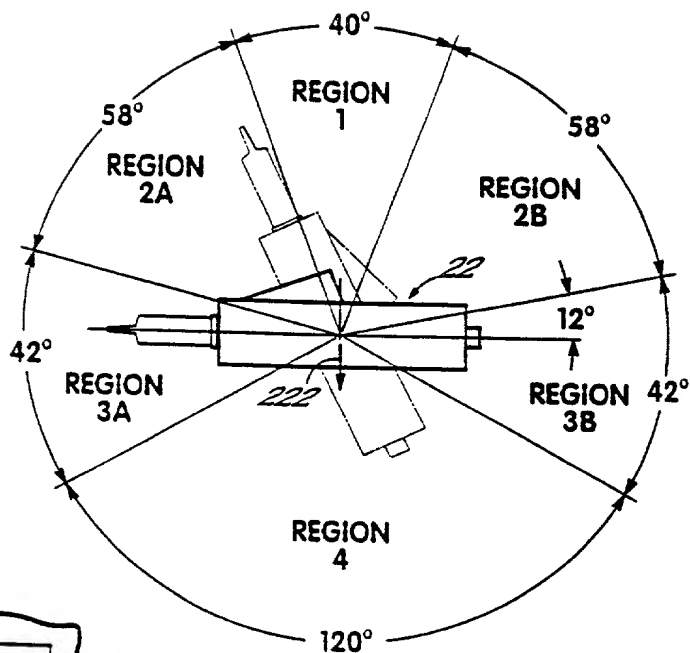


FIG. 13A

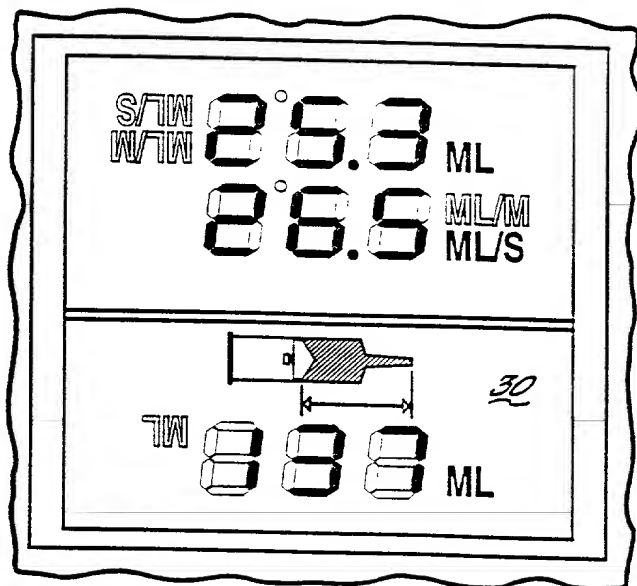


FIG. 13B

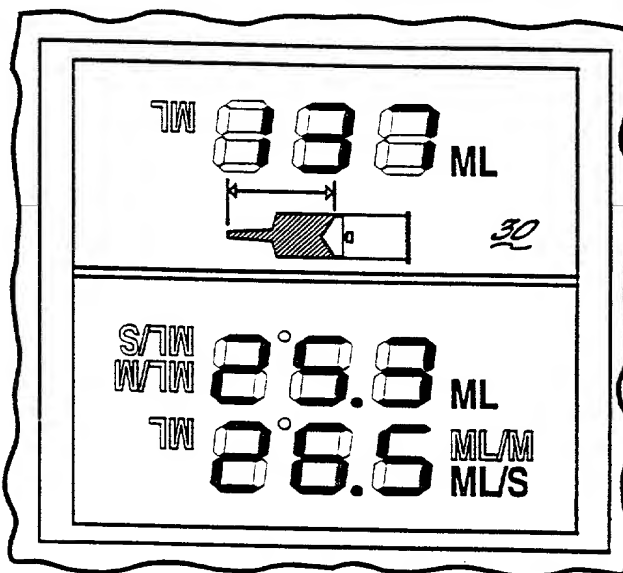


FIG. 13C

## DECLARATION, POWER OF ATTORNEY, AND PETITION

As a below named inventor, I hereby declare that:

My residence, post office address and citizenship are as stated below next to my name,

I believe I am the original, first and sole inventor (if only one name is listed below) or an original, first joint inventor (if plural names are listed below) of the subject matter which is claimed and for which a patent is sought on the invention entitled:

### MEDICAL FLUID INJECTOR

the specification of which was filed November 22, 1996, via Express Mail No. TB875325572US.

I hereby state that I have reviewed and understand the contents of the above identified specification, including the claims, as amended by any amendment referred to above.

I hereby acknowledge the duty to disclose to the United States Patent and Trademark Office all information known to me to be material to patentability as defined in Title 37, Code of Federal Regulations §1.56.

And, I hereby appoint John D. Poffenberger (R. No. 20,245), Bruce Tittel (R. No. 22,324), Donald F. Frei (R. No. 21,190), David J. Josephic (R. No. 22,849), A. Ralph Navaro, Jr. (R. No. 23,050), David S. Stallard (R. No. 25,930), J. Robert Chambers (R. No. 25,448), Gregory J. Lunn (R. No. 29,945), Kurt L. Grossman (R. No. 29,799), Clement H. Luken, Jr. (R. No. 32,742), Thomas J. Burger (R. No. 32,662), Gregory F. Ahrens (R. No. 32,957), Joseph R. Jordan (R. No. 25,686), Wayne L. Jacobs (R. No. 35,553), Kurt A. Summe (R. No. 36,023), Keith R. Haupt (R. No. 37,638), C. Richard Eby (R. No. 25,854), Theodore R. Remaklus (R. No. 38,754), Thomas W. Humphrey (R. No. 34,353), David E. Pritchard (R. No. 38,273), J. Dwight Poffenberger, Jr. (R. No. 35,324), Stephen W. Barns (R. No. 38,037) and, of counsel, Herbert C. Brinkman (R. No. 16,955) and Richard H. Evans (R. No. 19,755), in care of Wood, Herron & Evans, 2700 Carew Tower, Cincinnati, Ohio 45202, and telephone No. 513-241-2324, my attorneys/agents with full power of substitution and revocation, to prosecute this application and to transact all business in the Patent and Trademark Office connected therewith. All correspondence should be sent to Thomas W. Humphrey, Wood, Herron & Evans, 2700 Carew Tower, Cincinnati, Ohio 45202.

Wherefore I pray that Letter Patent be granted to me for the invention or discovery described and claimed in the foregoing specification and claims, and I hereby subscribe my name to the foregoing specification and claims, declaration, power of attorney, and this petition.

I hereby declare that all statements made herein of my own knowledge are true and that all statements made on information and belief are believed to be true; and further that these statements were made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment, or both, under Section 1001 of Title 18 of the United States Code and that such willful false statements may jeopardize the validity of the application or any patent issued thereon.

65337 "OFFICE"

Dane J. Battiato

Full name of inventor

*Dane J. Battiato*

12-12-96

Inventor's Signature

Date

U.S.A.

Citizenship

Cincinnati, Ohio

Residence

11343 Terwilliger's Valley Lane, Cincinnati, OH 45249

Post Office Address

Gary S. Wagner

Full name of inventor

*Gary S. Wagner*

12-12-96

Inventor's Signature

Date

U.S.A.

Citizenship

Taylor Mill, Kentucky

Residence

695 Arrowwood Circle, Taylor Mill, KY 41015

Post Office Address

Steve P. Verdino

Full name of inventor

*Steve P. Verdino*

16 DEC 96

Inventor's Signature

Date

U.S.A.

Citizenship

Cincinnati, Ohio

Residence

2781 Geraldine Drive, Cincinnati, OH 45239

Post Office Address

Robert G. Bergen

Full name of inventor

Inventor's Signature

Date

U.S.A.

Citizenship

Westchester, Ohio

Residence

7862 Willow Run Court, Westchester, OH 45069

Post Office Address

James E. Knipfer

Full name of inventor

Inventor's Signature

Date

U.S.A.

Citizenship

Ft. Wright, Kentucky

Residence

1238 Upland Avenue, Ft. Wright, KY 41011

Post Office Address

Pamela K. Jacobs

Full name of inventor

Inventor's Signature

Date

U.S.A.

Citizenship

Loveland, Ohio

Residence

10138 Fox Chase, Loveland, OH 45140

Post Office Address

65077-0746

65077-07460

Peter F. Staats

Full name of inventor

Peter F. Staats

Inventor's Signature

12/12/96

Date

U.S.A.

Citizenship

Loveland, Ohio

Residence

565 Belle Meade Drive, Loveland, OH 45140

Post Office Address

John N. Minnich

Full name of inventor

John N. Minnich

Inventor's Signature

12/12/1996

Date

U.S.A.

Citizenship

Lockland, Ohio

Residence

101 Eggerding Drive, Lockland, OH 45215

Post Office Address

Charles S. Neer

Full name of inventor

Charles S. Neer

Inventor's Signature

12-12-96

Date

U.S.A.

Citizenship

Milford, Ohio

Residence

949 Tarragon Lane, Milford, OH 45150

Post Office Address

James H. Goethel

Full name of inventor

James H. Goethel

12/15/94

Inventor's Signature

Date

U.S.A.

Citizenship

Cincinnati, Ohio

Residence

9966 Thornwood Court, Cincinnati, OH 45241

Post Office Address

Mitchell G. Stern

Full name of inventor



Inventor's Signature

12/12/96

Date

U.S.A.

Citizenship

Centerville, Ohio

Residence

7871 Millerton Drive, Centerville, OH 45459

Post Office Address